

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110521\
 Data File : VW023224.D
 Acq On : 05 Nov 2021 12:03
 Operator : SY/MD
 Sample : M4464-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L7

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021
 Supervised By :Semsettin Yesilyurt 11/20/2021

Quant Time: Nov 10 09:35:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	139071	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	139269	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69198	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	39358	4.518	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.400%
7) Chloroethane-d5	1.567	69	33635	4.737	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.108	63	71130	4.361	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.200%
20) 2-Butanone-d5	3.908	46	68446	45.601	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.200%
24) Chloroform-d	4.349	84	85579	4.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	5.034	65	40695	4.874	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
32) Benzene-d6	5.050	84	168813	4.724	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	6.072	67	49547	4.710	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.200%
41) Toluene-d8	7.316	98	141253	4.218	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
43) trans-1,3-Dichloroprop...	7.628	79	17951	4.501	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.091	63	74860	51.011	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36479	4.822	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	57284	4.972	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.400%
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	42141	3.655	ug/L	96
6) Bromomethane	1.522	94	23181	3.149	ug/L	100
9) Trichlorofluoromethane	1.754	101	130869	7.564	ug/L	100
12) 1,1-Dichloroethene	2.117	96	30993	3.737	ug/L	96
13) Acetone	2.198	43	98677m	107.593	ug/L	
14) Carbon disulfide	2.294	76	161379	5.156	ug/L	99
16) Methylene chloride	2.506	84	26520	2.191	ug/L	91
17) Methyl tert-butyl Ether	2.770	73	170798	9.356	ug/L	96
19) 1,1-Dichloroethane	3.191	63	166160	9.653	ug/L	98
21) 2-Butanone	3.982	43	204329m	137.801	ug/L	
27) 1,2-Dichloroethane	5.133	62	74576	7.642	ug/L	99
29) 1,1,1-Trichloroethane	4.609	97	149488	8.838	ug/L	99
30) Cyclohexane	4.680	56	178861	11.801	ug/L	96
34) Trichloroethene	5.915	95	66073	6.383	ug/L	99
35) Methylcyclohexane	6.133	83	108284	6.628	ug/L	97
37) 1,2-Dichloropropane	6.175	63	19924	2.192	ug/L	99
42) Toluene	7.387	91	372692	8.952	ug/L	99
47) Tetrachloroethene	7.976	164	80635	8.988	ug/L	99
48) 2-Hexanone	8.143	43	212589	71.984	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023224.D
 Acq On : 05 Nov 2021 12:03
 Operator : SY/MD
 Sample : M4464-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L7

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021
 Supervised By :Semsettin Yesilyurt 11/20/2021

Quant Time: Nov 10 09:35:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 10 00:38:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

50) 1,2-Dibromoethane	8.352	107	101831	16.829	ug/L	96
51) Chlorobenzene	8.882	112	308819	11.159	ug/L	99
52) Ethylbenzene	9.014	91	316061	7.198	ug/L	97
53) m,p-xylene	9.143	106	250697	14.547	ug/L	97
54) o-xylene	9.545	106	94420	5.840	ug/L	99
55) Styrene	9.561	104	163187	5.892	ug/L	99
59) Bromoform	9.731	173	24575	5.946	ug/L	98
60) Isopropylbenzene	9.934	105	155667	3.920	ug/L	99
65) 1,4-Dichlorobenzene	11.271	146	95459	4.607	ug/L	98
67) 1,2-Dichlorobenzene	11.644	146	250482	13.797	ug/L	99
68) 1,2-Dibromo-3-chloropr...	12.429	75	4564	4.660	ug/L	88
72) 1,2,3-Trichlorobenzene	13.744	180	131123	11.780	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

TIC: VV023224.D\data.ms

Abundance

Time-->

Chloromethane-d3, S
Chloromethane, S
Trichlorofluoromethane, T
Acetone, T
Carbon disulfide, T
Methylene chloride, T
Methyl tert-butyl Ether, T
1,1-Dichloroethane, T
2-Butanone-d6, S
Chloroform-d3
1,1,1-Trichloroethane, T
Cyclohexane, T
1,2-Dichloroethane, T
1,2-Dichloropropane, T
1,4-Difluorobenzene, I
Trichloroethene, T
1,2-Dichloropropane-d5, S
Methylcyclohexane, T
Toluene, T
trans-1,3-Dichloropropene-d4, S
Toluene-d8, S
Tetrachloroethene, T
2-Hexanone-d5, S
2-Hexanone, T
1,2-Dibromoethane, T
Chlorobenzene-d5, I
Chlorobenzene, T
Ethylbenzene, T
m,p-xylene, T
Styrene, T
Isopropylbenzene, T
1,1,2,2-Tetrachloroethane-d2, S
Bromoforn, T
1,2-Dibromo-3-chloropropane, T
1,4-Dichlorobenzene-d4, I
1,4-Dichlorobenzene, T
1,2-Dichlorobenzene-d4, S
1,2-Dichlorobenzene, T
1,2,3-Trichlorobenzene, T

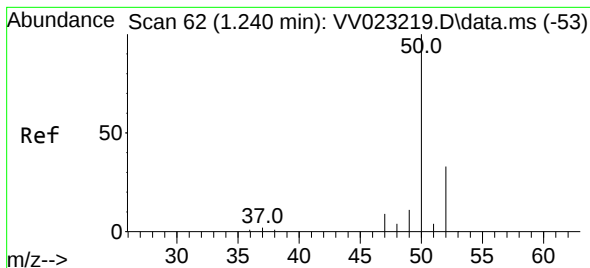

#3

Chloromethane

Concen: 3.655 ug/L

RT: 1.240 min Scan# 61

Delta R.T. -0.000 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 50 Resp: 4214

Ion Ratio Lower Upper

50 100





52 32.2 24.3 45.1

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021

Supervised By :Semsettin Yesilyurt 11/20/2021

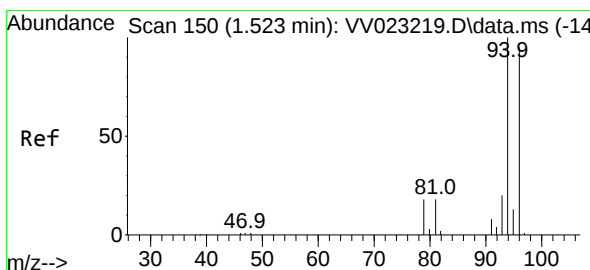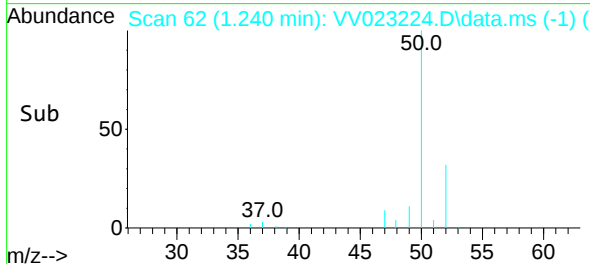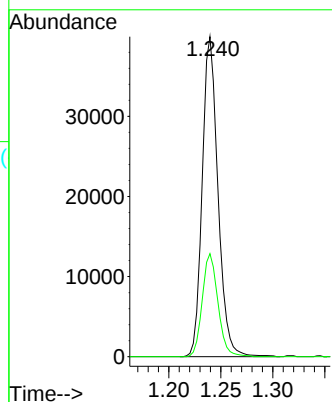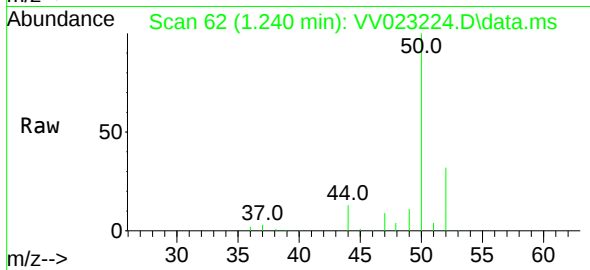

#6

Bromomethane

Concen: 3.149 ug/L

RT: 1.522 min Scan# 150

Delta R.T. 0.003 min

Lab File: VV023224.D




Acq: 05 Nov 2021 12:03


Tgt Ion: 94 Resp: 23181

Ion Ratio Lower Upper

94 100


96 93.0 65.0 120.8

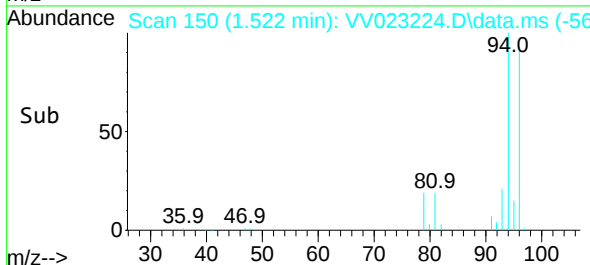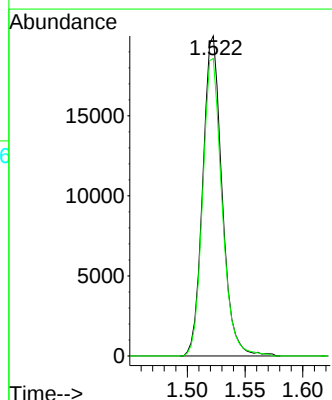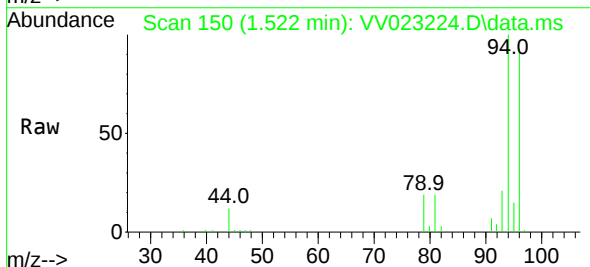



#9
 Trichlorofluoromethane
 Concen: 7.564 ug/L
 RT: 1.754 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV023224.D
 Acq: 05 Nov 2021 12:03




Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L7

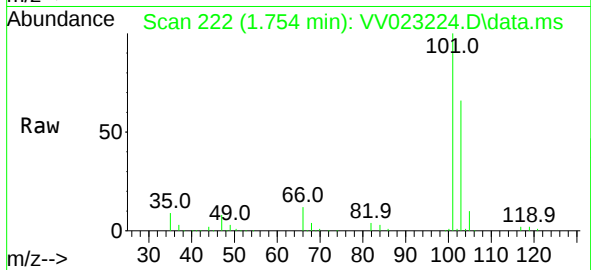


Tgt Ion:101 Resp: 130869
 Ion Ratio Lower Upper
 101 100
 103 65.4 52.6 79.0

Manual Integrations
 APPROVED



Reviewed By :Mahesh Dadoda 11/20/2021
 Supervised By :Semsettin Yesilyurt 11/20/2021

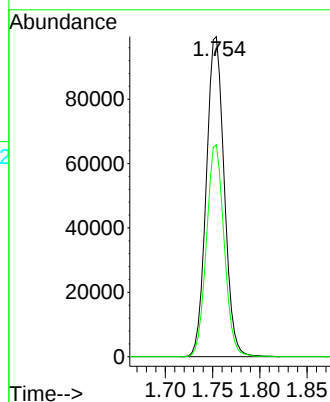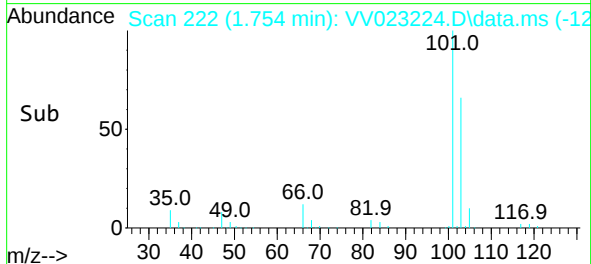


#12
 1,1-Dichloroethene
 Concen: 3.737 ug/L
 RT: 2.117 min Scan# 335
 Delta R.T. -0.000 min
 Lab File: VV023224.D
 Acq: 05 Nov 2021 12:03

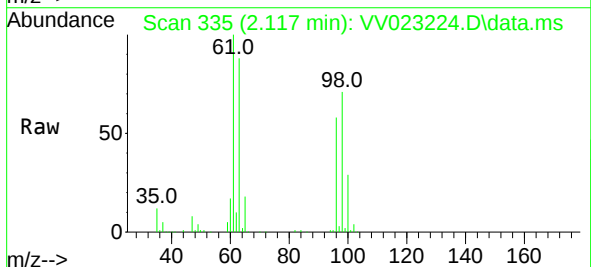


Tgt Ion: 96 Resp: 30993
 Ion Ratio Lower Upper
 96 100
 61 173.5 121.5 225.7
 63 152.9 99.6 185.0





#13
Acetone
Concen: 107.593 ug/L m
RT: 2.198 min Scan# 30
Delta R.T. 0.006 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7



Tgt Ion: 43 Resp: 9867
Ion Ratio Lower Upper
43 100
58 21.5 0.0 55.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

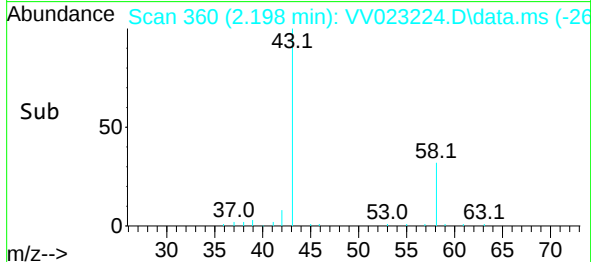

#14
Carbon disulfide
Concen: 5.156 ug/L
RT: 2.294 min Scan# 390
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03


Tgt Ion: 76 Resp: 161379
Ion Ratio Lower Upper
76 100
78 9.5 7.2 10.8

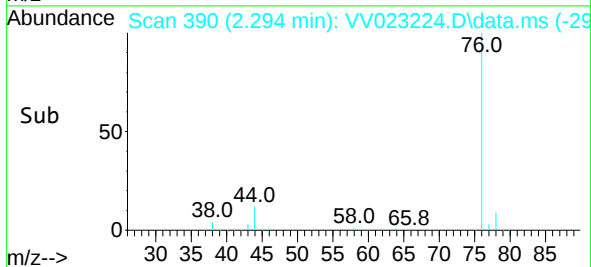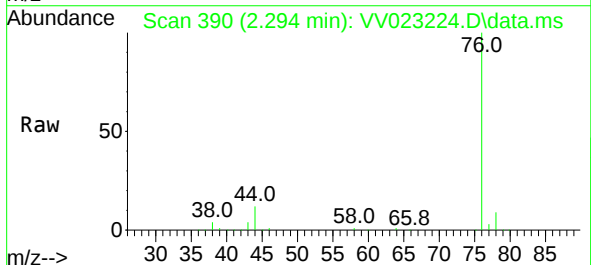



#16
Methylene chloride
Concen: 2.191 ug/L
RT: 2.506 min Scan# 456
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7



Tgt Ion: 84 Resp: 26520
Ion Ratio Lower Upper
84 100
86 66.9 42.3 78.5
49 123.1 79.7 148.1




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021



#17
Methyl tert-butyl Ether
Concen: 9.356 ug/L
RT: 2.770 min Scan# 538
Delta R.T. 0.003 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

Tgt Ion: 73 Resp: 170798
Ion Ratio Lower Upper
73 100
43 18.8 17.4 26.0
57 21.9 16.5 24.7

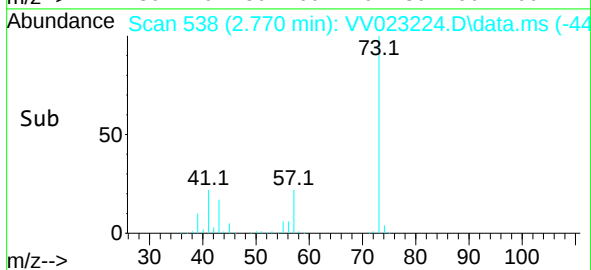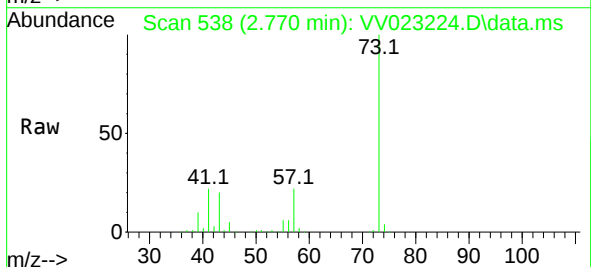



#19

1,1-Dichloroethane

Concen: 9.653 ug/L

RT: 3.191 min Scan# 6

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 63 Resp: 166160

Ion Ratio Lower Upper

63 100

65 32.3 22.6 42.0





83 13.9 11.1 20.7

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021

Supervised By :Semsettin Yesilyurt 11/20/2021

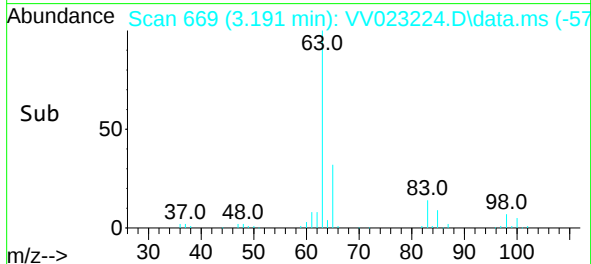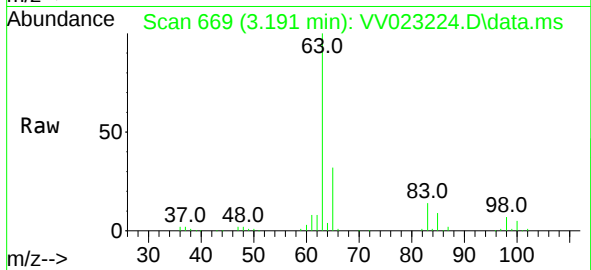

#21

2-Butanone

Concen: 137.801 ug/L m

RT: 3.982 min Scan# 915

Delta R.T. -0.000 min

Lab File: VV023224.D




Acq: 05 Nov 2021 12:03


Tgt Ion: 43 Resp: 204329

Ion Ratio Lower Upper

43 100

72 23.3 11.9 35.9

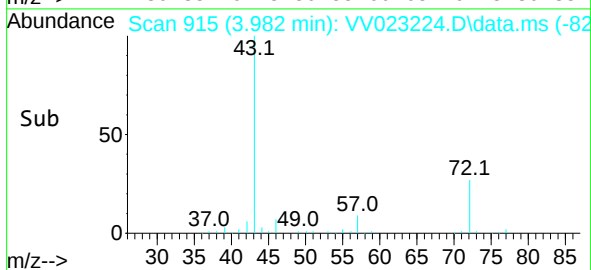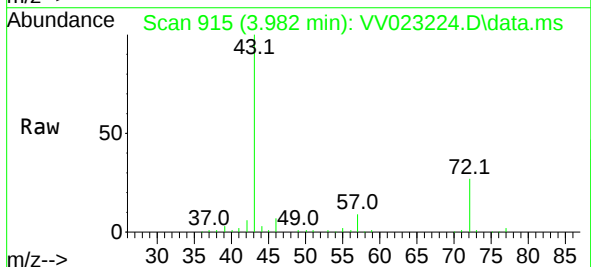



#27

1,2-Dichloroethane

Concen: 7.642 ug/L

RT: 5.133 min Scan# 11

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 62 Resp: 74570

Ion Ratio Lower Upper

62 100





98 9.9 8.2 12.4

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021

Supervised By :Semsettin Yesilyurt 11/20/2021



#29

1,1,1-Trichloroethane

Concen: 8.838 ug/L

RT: 4.609 min Scan# 1110

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03




Tgt Ion: 97 Resp: 149488


Ion Ratio Lower Upper

97 100

99 64.1 51.0 76.4

61 41.7 34.1 51.1

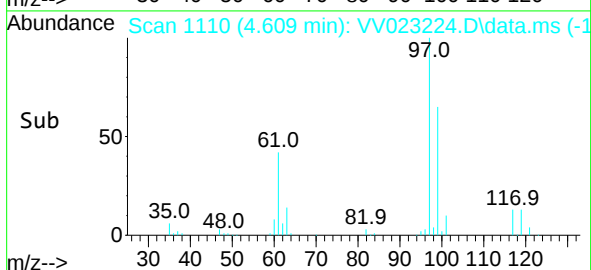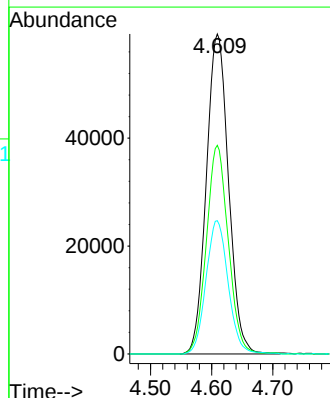



#30

Cyclohexane

Concen: 11.801 ug/L

RT: 4.680 min Scan# 1131

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 56 Resp: 17886

Ion Ratio Lower Upper

56 100





69 31.2 23.5 35.3

84 94.0 71.6 107.4

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

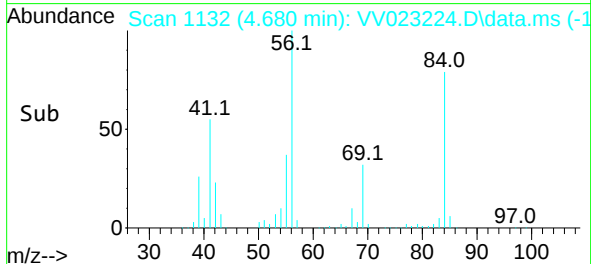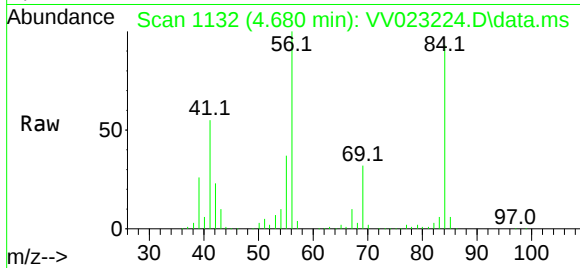

#34

Trichloroethene

Concen: 6.383 ug/L

RT: 5.915 min Scan# 1516

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Tgt Ion: 95 Resp: 66073




Ion Ratio Lower Upper


95 100

97 64.0 45.0 83.6

132 102.3 69.7 129.4

130 104.8 73.7 136.9

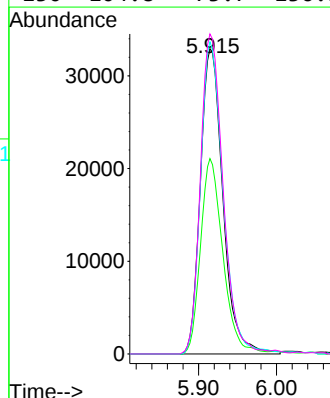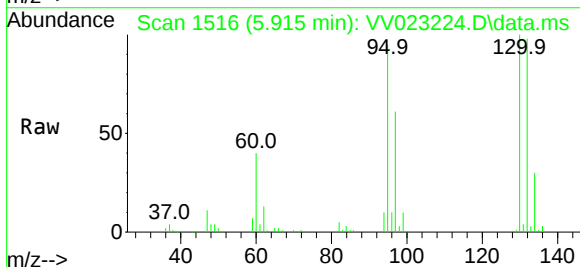

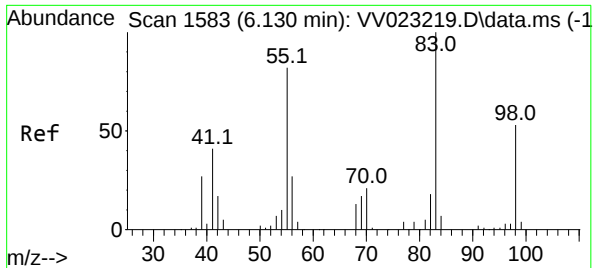

#35

Methylcyclohexane

Concen: 6.628 ug/L

RT: 6.133 min Scan# 1583

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 83 Resp: 108284

Ion Ratio Lower Upper

83 100

55 75.6 62.8 94.2





98 49.8 37.9 56.9

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021

Supervised By :Semsettin Yesilyurt 11/20/2021

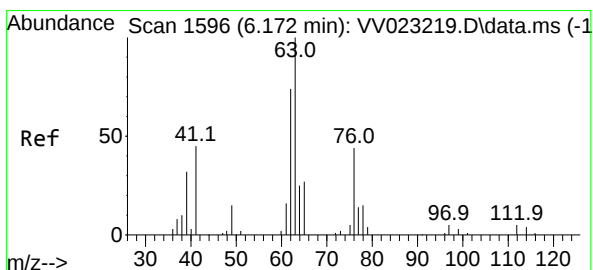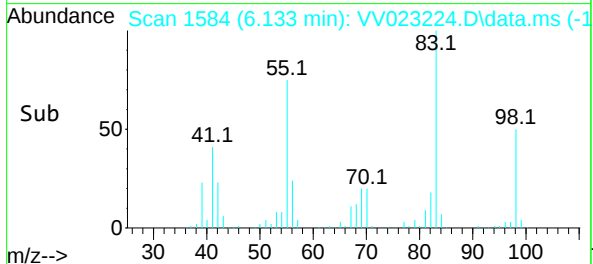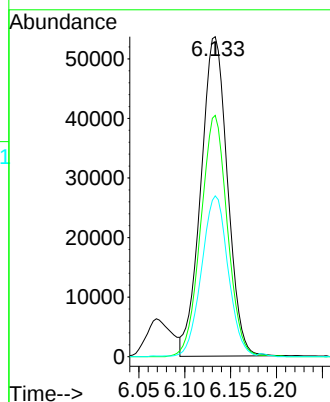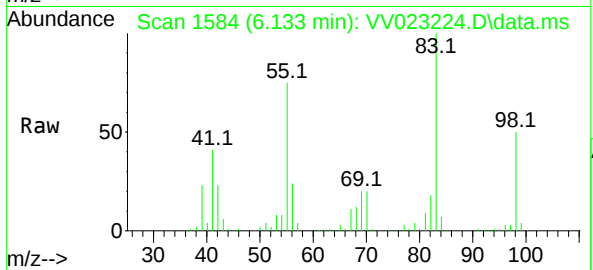

#37

1,2-Dichloropropane

Concen: 2.192 ug/L

RT: 6.175 min Scan# 1597

Delta R.T. 0.003 min

Lab File: VV023224.D




Acq: 05 Nov 2021 12:03


Tgt Ion: 63 Resp: 19924

Ion Ratio Lower Upper

63 100

112 5.3 4.6 6.8

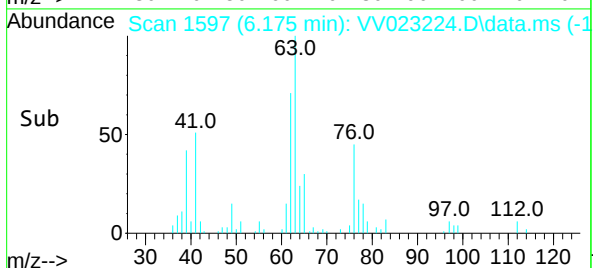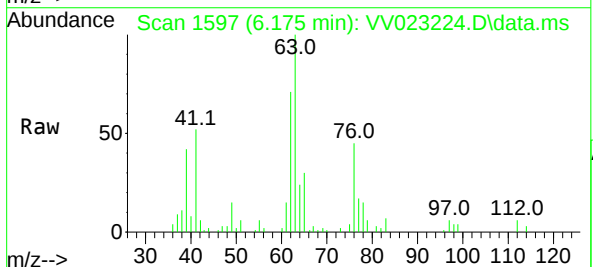

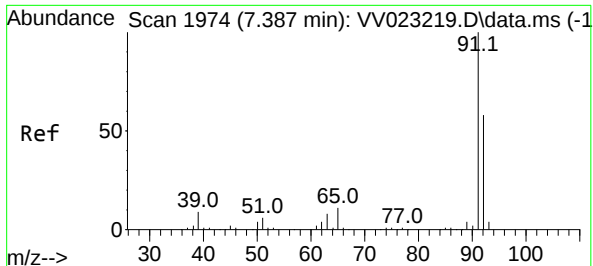

#42

Toluene

Concen: 8.952 ug/L

RT: 7.387 min Scan# 1974

Delta R.T. -0.000 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Instrument :

MSVOA_V

ClientSampleId :

GB7L7

Tgt Ion: 91 Resp: 372692

Ion Ratio Lower Upper

91 100





92 57.0 39.3 72.9

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021

Supervised By :Semsettin Yesilyurt 11/20/2021

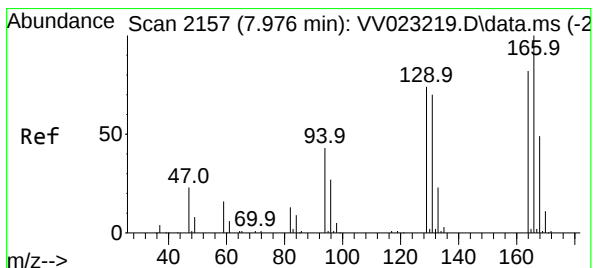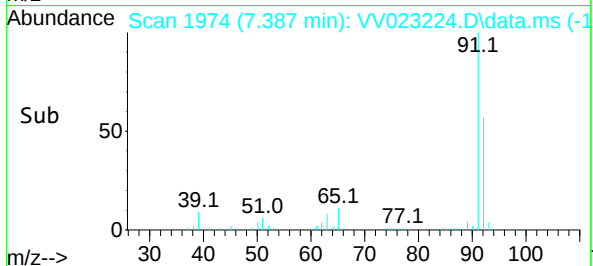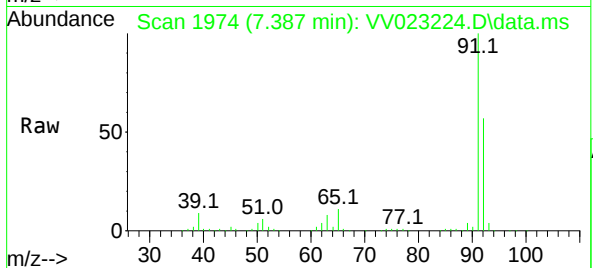

#47

Tetrachloroethene

Concen: 8.988 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. 0.003 min

Lab File: VV023224.D

Acq: 05 Nov 2021 12:03

Tgt Ion:164 Resp: 80635




Ion Ratio Lower Upper


164 100

129 92.9 64.0 119.0

131 88.6 63.4 117.8


166 127.0 89.3 165.9

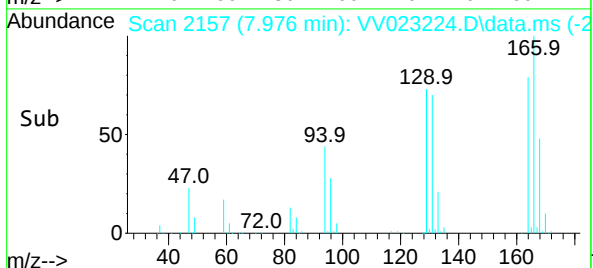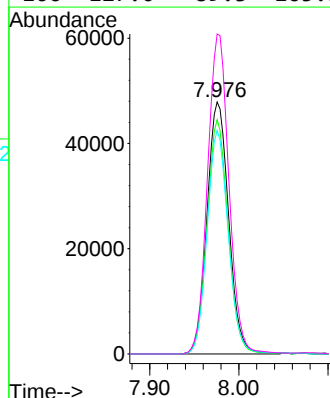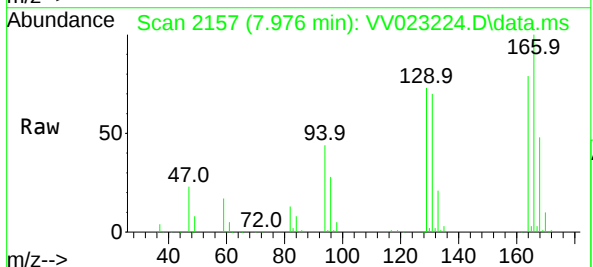



#48
2-Hexanone
Concen: 71.984 ug/L
RT: 8.143 min Scan# 212589
Delta R.T. 0.003 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7




Tgt Ion: 43 Resp: 212589
Ion Ratio Lower Upper
43 100
58 55.2 43.7 65.5
57 19.3 14.1 21.1
100 13.4 10.2 15.2

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

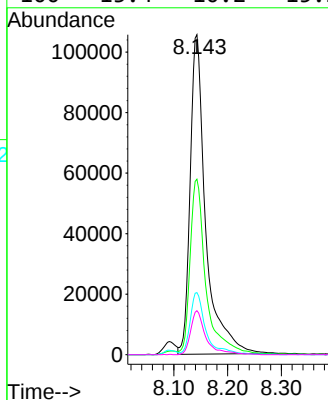


#50
1,2-Dibromoethane
Concen: 16.829 ug/L
RT: 8.352 min Scan# 2274
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

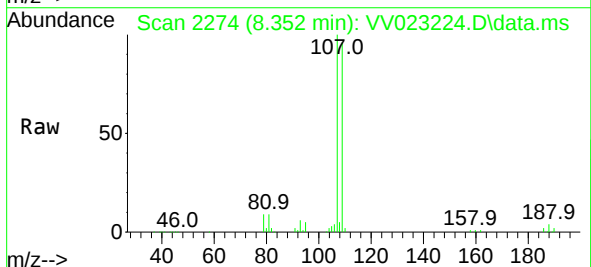


Tgt Ion:107 Resp: 101831
Ion Ratio Lower Upper
107 100
109 95.9 64.7 120.1
188 4.2 3.6 5.4

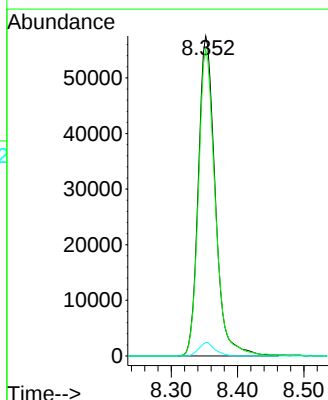



#51
Chlorobenzene
Concen: 11.159 ug/L
RT: 8.882 min Scan# 2439
Delta R.T. 0.003 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7



Tgt Ion:112 Resp: 308819
Ion Ratio Lower Upper
112 100
114 31.8 22.0 40.8
77 54.4 44.4 66.6




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

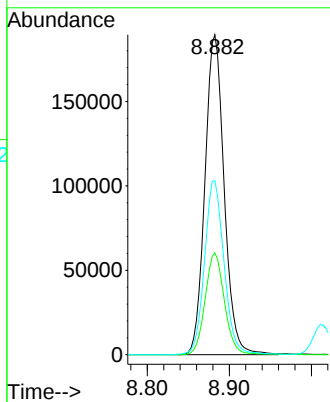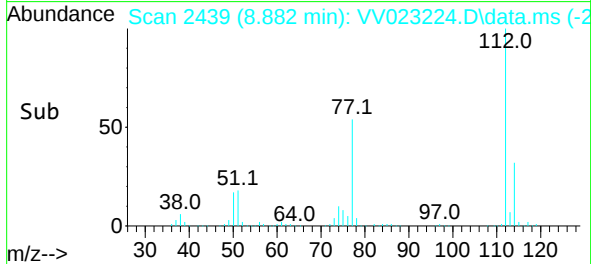

#52
Ethylbenzene
Concen: 7.198 ug/L
RT: 9.014 min Scan# 2480
Delta R.T. 0.003 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

Tgt Ion: 91 Resp: 316061
Ion Ratio Lower Upper
91 100
106 30.2 22.5 41.9

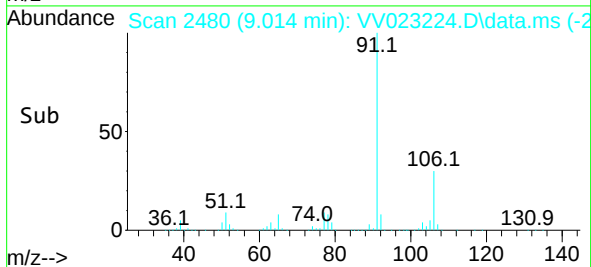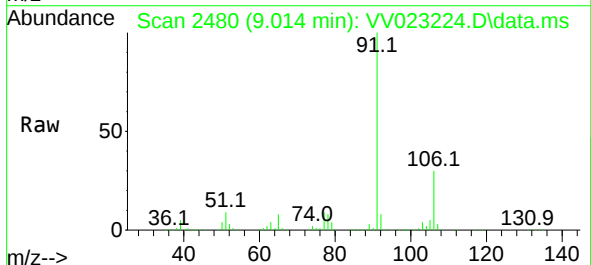







#53
m,p-xylene
Concen: 14.547 ug/L
RT: 9.143 min Scan# 21
Delta R.T. 0.006 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

Instrument :
MSVOA_V
ClientSampleId :
GB7L7

Tgt Ion:106 Resp: 25069
Ion Ratio Lower Upper
106 100
91 200.8 137.2 254.8




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

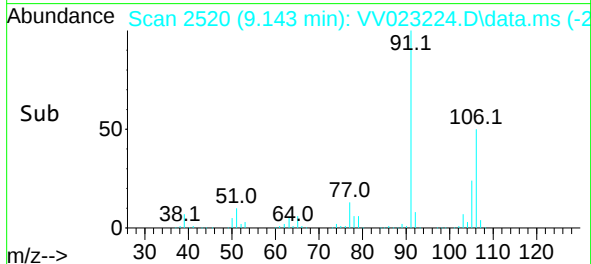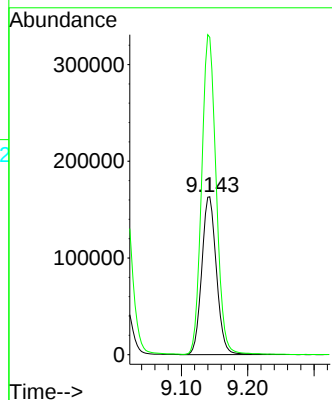

#54
o-xylene
Concen: 5.840 ug/L
RT: 9.545 min Scan# 2645
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03


Tgt Ion:106 Resp: 94420
Ion Ratio Lower Upper
106 100
91 213.0 148.3 275.5

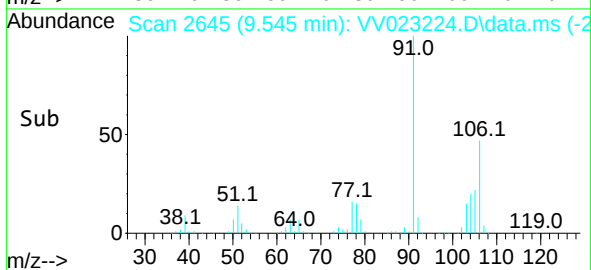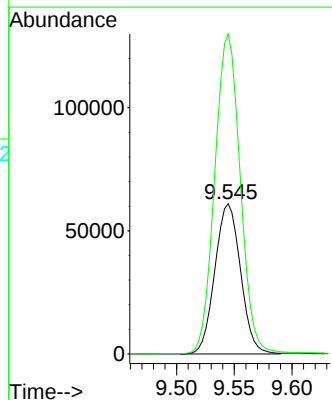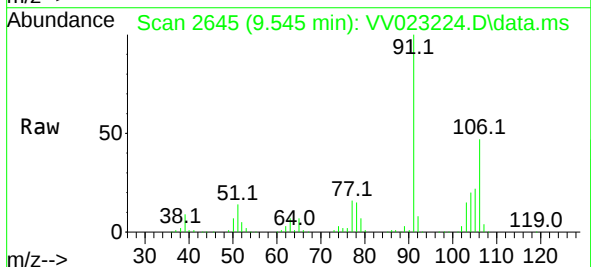

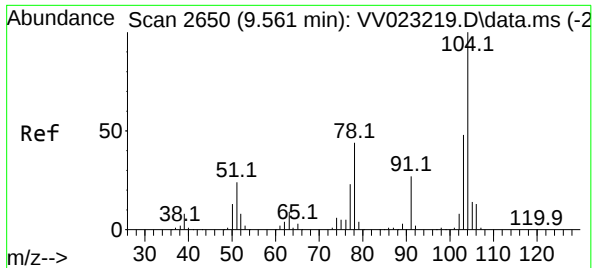

#55
Styrene
Concen: 5.892 ug/L
RT: 9.561 min Scan# 2703
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7

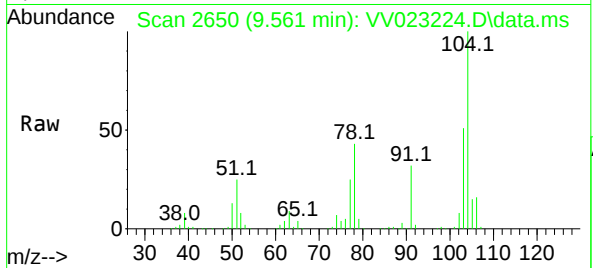

Tgt Ion:104 Resp: 16318
Ion Ratio Lower Upper
104 100
78 42.7 29.3 54.3




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

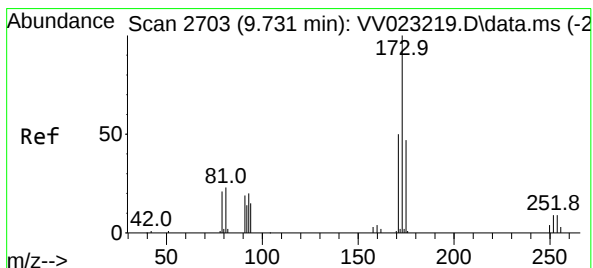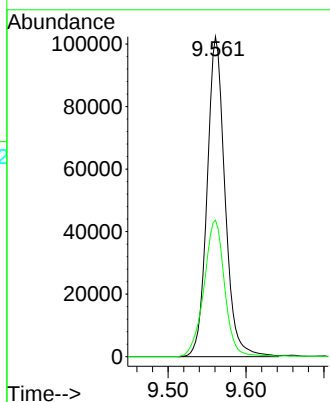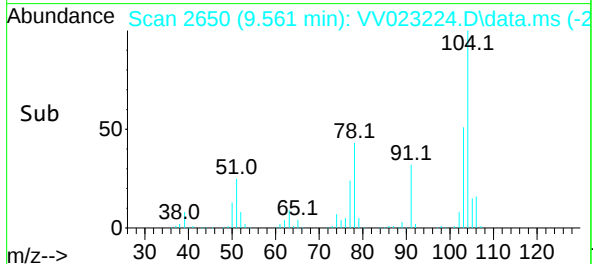

#59
Bromoform
Concen: 5.946 ug/L
RT: 9.731 min Scan# 2703
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03


Tgt Ion:173 Resp: 24575
Ion Ratio Lower Upper
173 100
175 48.7 38.2 57.2
254 8.8 6.2 9.2

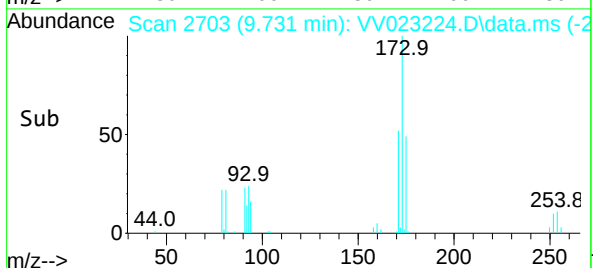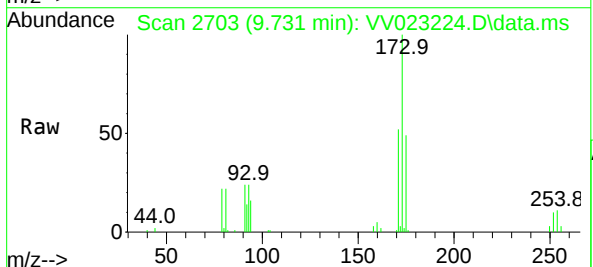



#60
Isopropylbenzene
Concen: 3.920 ug/L
RT: 9.934 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03




Instrument :
MSVOA_V
ClientSampleId :
GB7L7

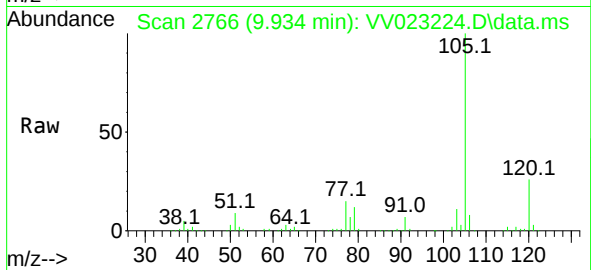


Tgt Ion:105 Resp: 15566
Ion Ratio Lower Upper
105 100
120 26.5 21.7 32.5
77 15.1 12.6 19.0

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

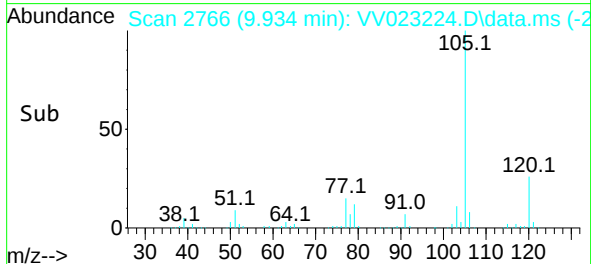


#65
1,4-Dichlorobenzene
Concen: 4.607 ug/L
RT: 11.271 min Scan# 3182
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

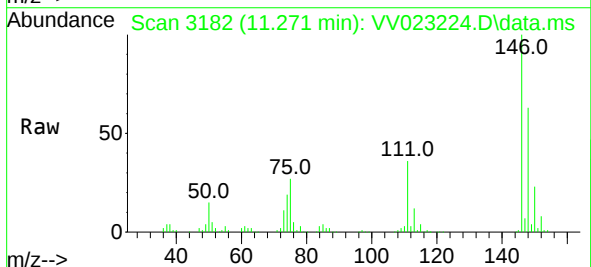

Tgt Ion:146 Resp: 95459
Ion Ratio Lower Upper
146 100
111 36.0 26.2 48.8
148 62.7 44.4 82.5

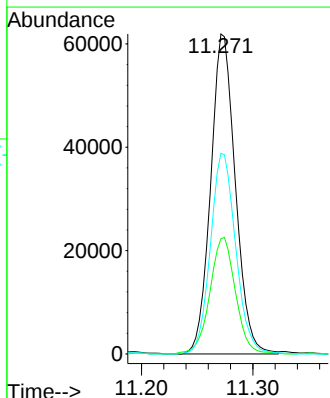







#67
1,2-Dichlorobenzene
Concen: 13.797 ug/L
RT: 11.644 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03

Instrument :
MSVOA_V
ClientSampleId :
GB7L7

Tgt Ion:146 Resp: 25048
Ion Ratio Lower Upper
146 100
111 40.5 31.6 47.4
148 64.1 51.0 76.6




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/20/2021
Supervised By :Semsettin Yesilyurt 11/20/2021

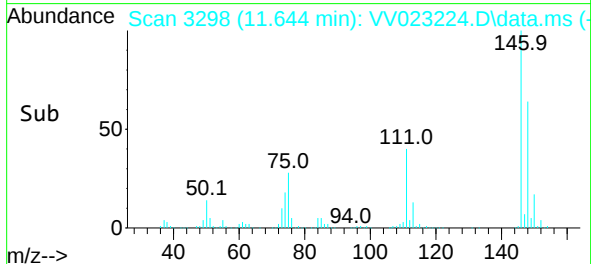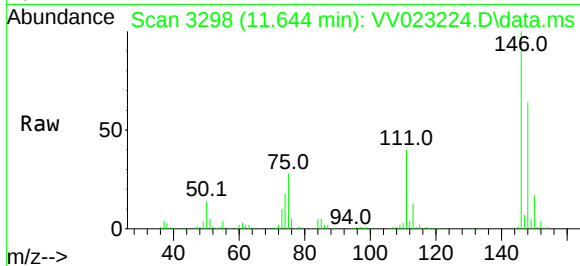

#68
1,2-Dibromo-3-chloropropane
Concen: 4.660 ug/L
RT: 12.429 min Scan# 3542
Delta R.T. -0.000 min
Lab File: VV023224.D
Acq: 05 Nov 2021 12:03


Tgt Ion: 75 Resp: 4564
Ion Ratio Lower Upper
75 100
155 81.9 67.7 101.5
157 130.4 87.9 131.9

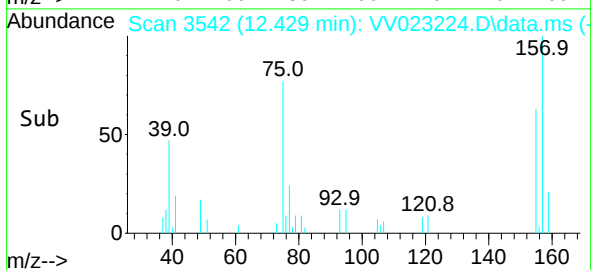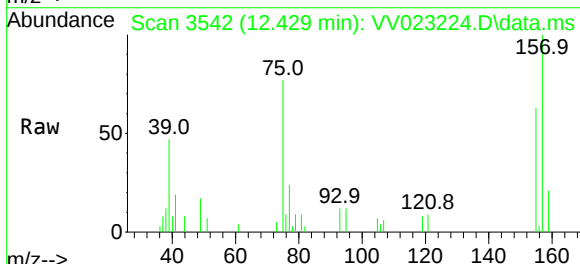

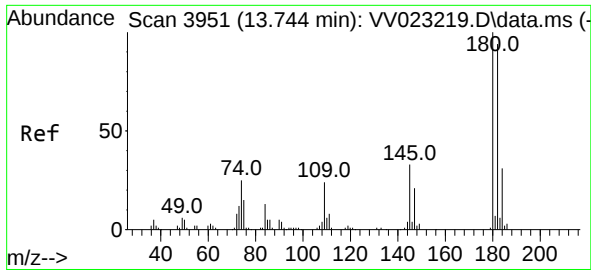

#72
 1,2,3-Trichlorobenzene
 Concen: 11.780 ug/L
 RT: 13.744 min Scan# 3951
 Delta R.T. -0.000 min
 Lab File: VV023224.D
 Acq: 05 Nov 2021 12:03

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L7

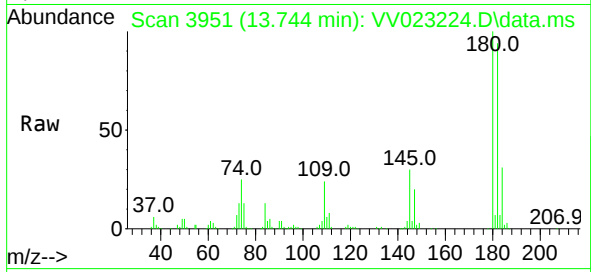

Tgt Ion:180 Resp: 131123
 Ion Ratio Lower Upper
 180 100
 182 94.1 76.7 115.1
 145 30.8 25.7 38.5

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 11/20/2021
 Supervised By :Semsettin Yesilyurt 11/20/2021

