

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110521\
 Data File : VW023233.D
 Acq On : 05 Nov 2021 15:37
 Operator : SY/MD
 Sample : M4464-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L6

Quant Time: Nov 09 03:11:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 02:04:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133863	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	134704	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63241	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	37457	4.467	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%
7) Chloroethane-d5	1.568	69	32167	4.706	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.200%
11) 1,1-Dichloroethene-d2	2.108	63	53865	3.431	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	3.896	46	75350	52.154	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.300%
24) Chloroform-d	4.349	84	82723	4.629	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.034	65	39460	4.910	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.053	84	158369	4.582	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.072	67	48348	4.752	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.317	98	134983	4.168	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.400%
43) trans-1,3-Dichloroprop...	7.625	79	16760	4.344	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.092	63	60404	42.555	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29822	4.076	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	51276	4.869	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds					Qvalue	
13) Acetone	2.182	43	2590	2.934	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023233.D
Acq On : 05 Nov 2021 15:37
Operator : SY/MD
Sample : M4464-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7L6

Quant Time: Nov 09 03:11:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 02:04:24 2021
Response via : Initial Calibration

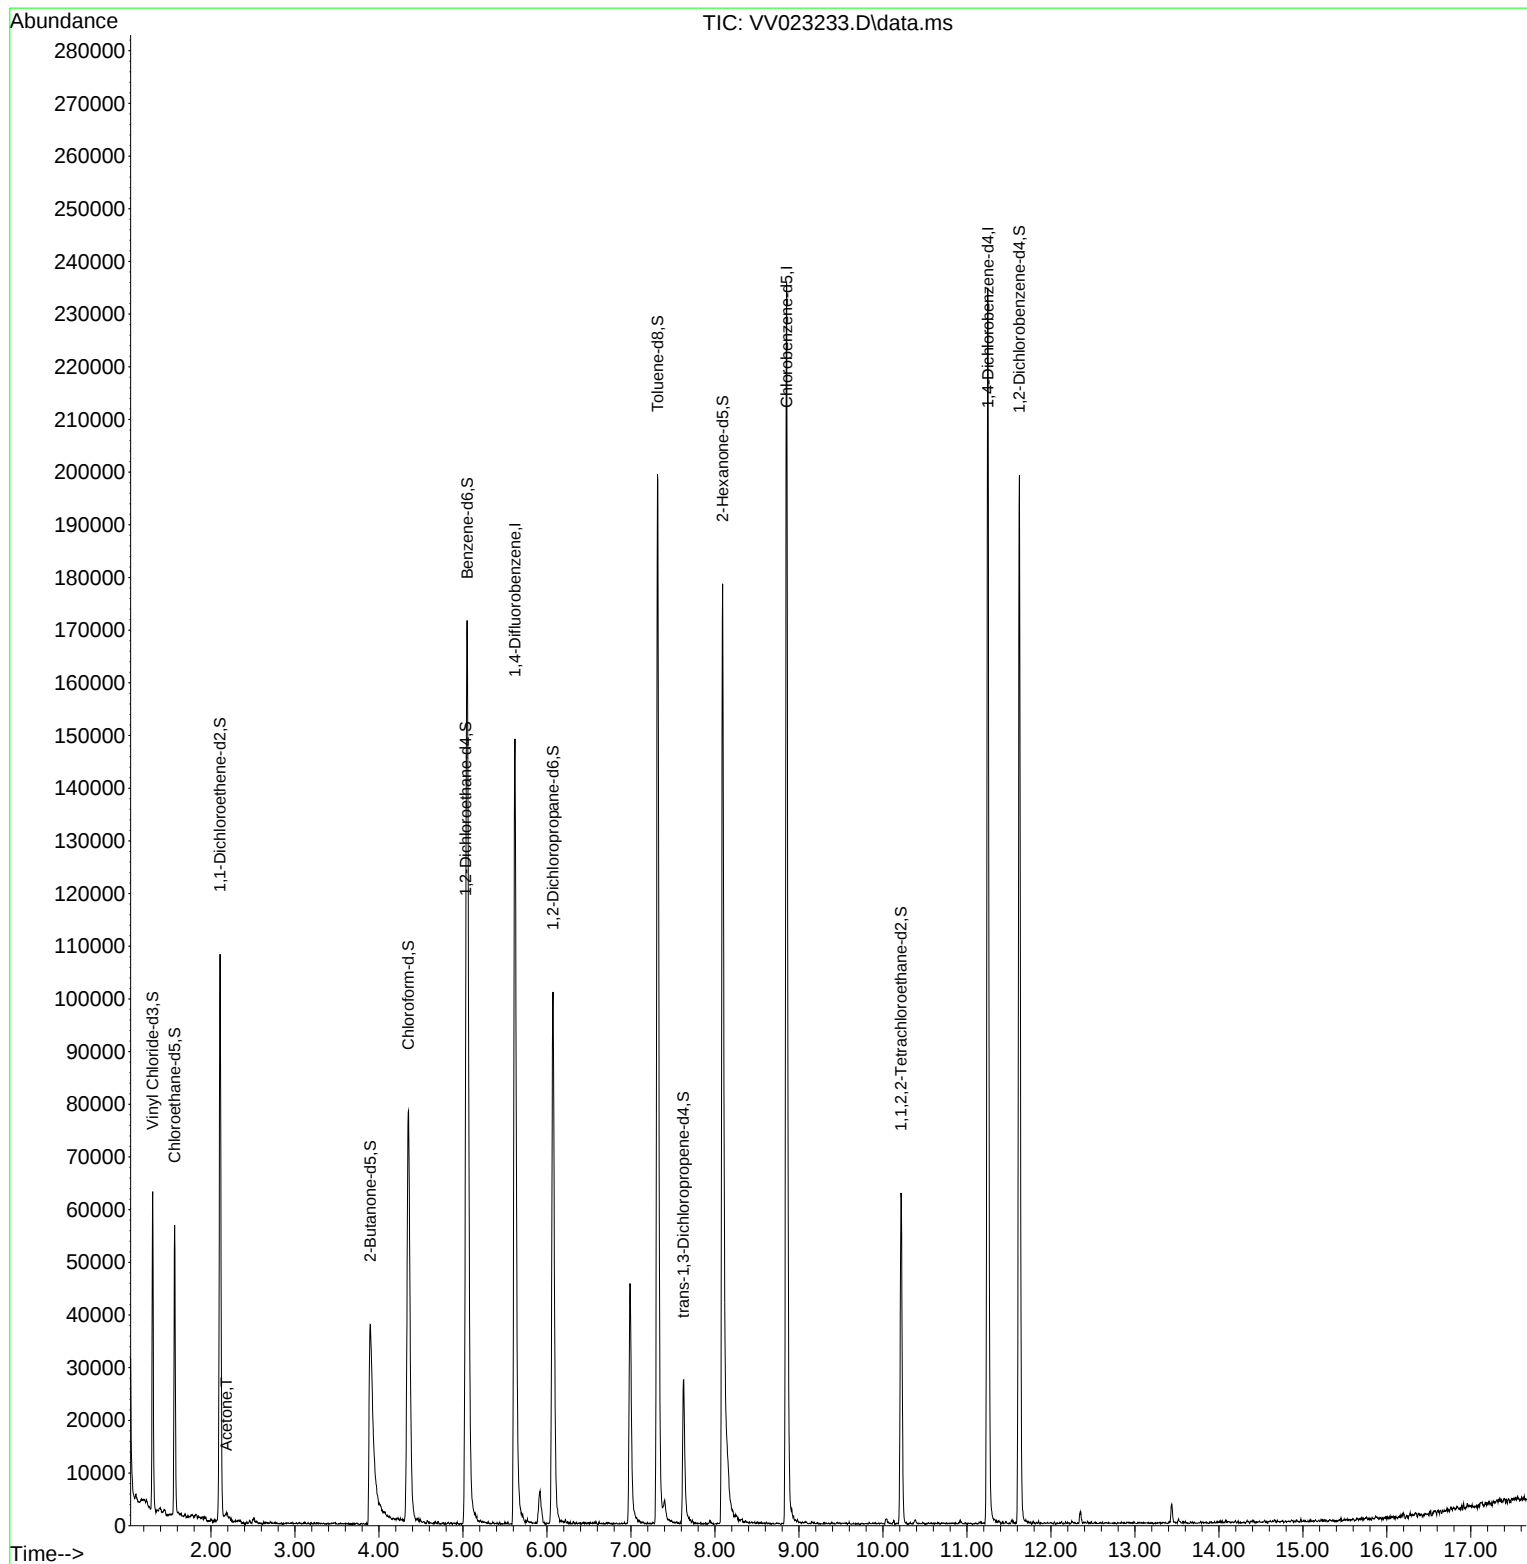

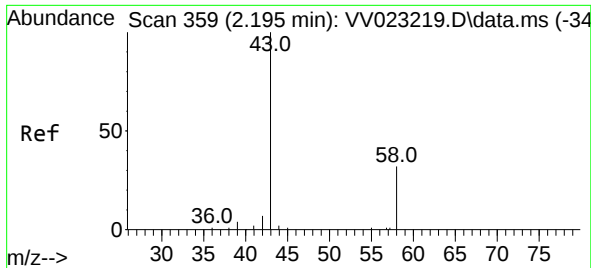

#13

Acetone

Concen: 2.934 ug/L

RT: 2.182 min Scan# 31

Delta R.T. -0.013 min

Lab File: VV023233.D


Acq: 05 Nov 2021 15:37

Instrument :

MSVOA_V

ClientSampleId :

GB7L6

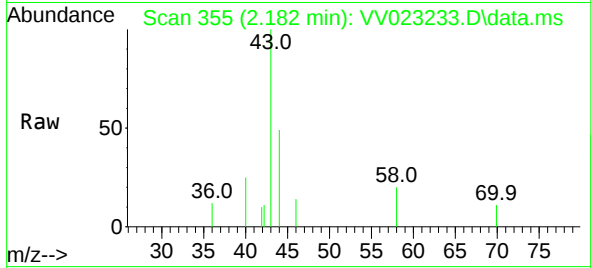

Tgt Ion: 43 Resp: 2590

Ion Ratio Lower Upper

43 100

58 23.1 0.0 55.4

