

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023249.D
 Acq On : 05 Nov 2021 22:15
 Operator : SY/MD
 Sample : M4535-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4570

Quant Time: Nov 09 04:06:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 03:48:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129996	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	130242	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59468	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36377	4.467	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.568	69	31731	4.781	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.111	63	51922	3.406	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.200%	
20) 2-Butanone-d5	3.889	46	79841	56.906	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	113.820%	
24) Chloroform-d	4.352	84	79242	4.566	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
26) 1,2-Dichloroethane-d4	5.034	65	38014	4.871	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
32) Benzene-d6	5.053	84	150639	4.508	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	6.072	67	47026	4.780	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.600%	
41) Toluene-d8	7.317	98	129158	4.124	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.625	79	16064	4.307	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.200%	
46) 2-Hexanone-d5	8.088	63	55301	40.295	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.580%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28495	4.028	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	80.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	50410	5.091	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.800%	
Target Compounds					Qvalue	
13) Acetone	2.182	43	6352	7.409	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023249.D
Acq On : 05 Nov 2021 22:15
Operator : SY/MD
Sample : M4535-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4570

Quant Time: Nov 09 04:06:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 03:48:20 2021
Response via : Initial Calibration

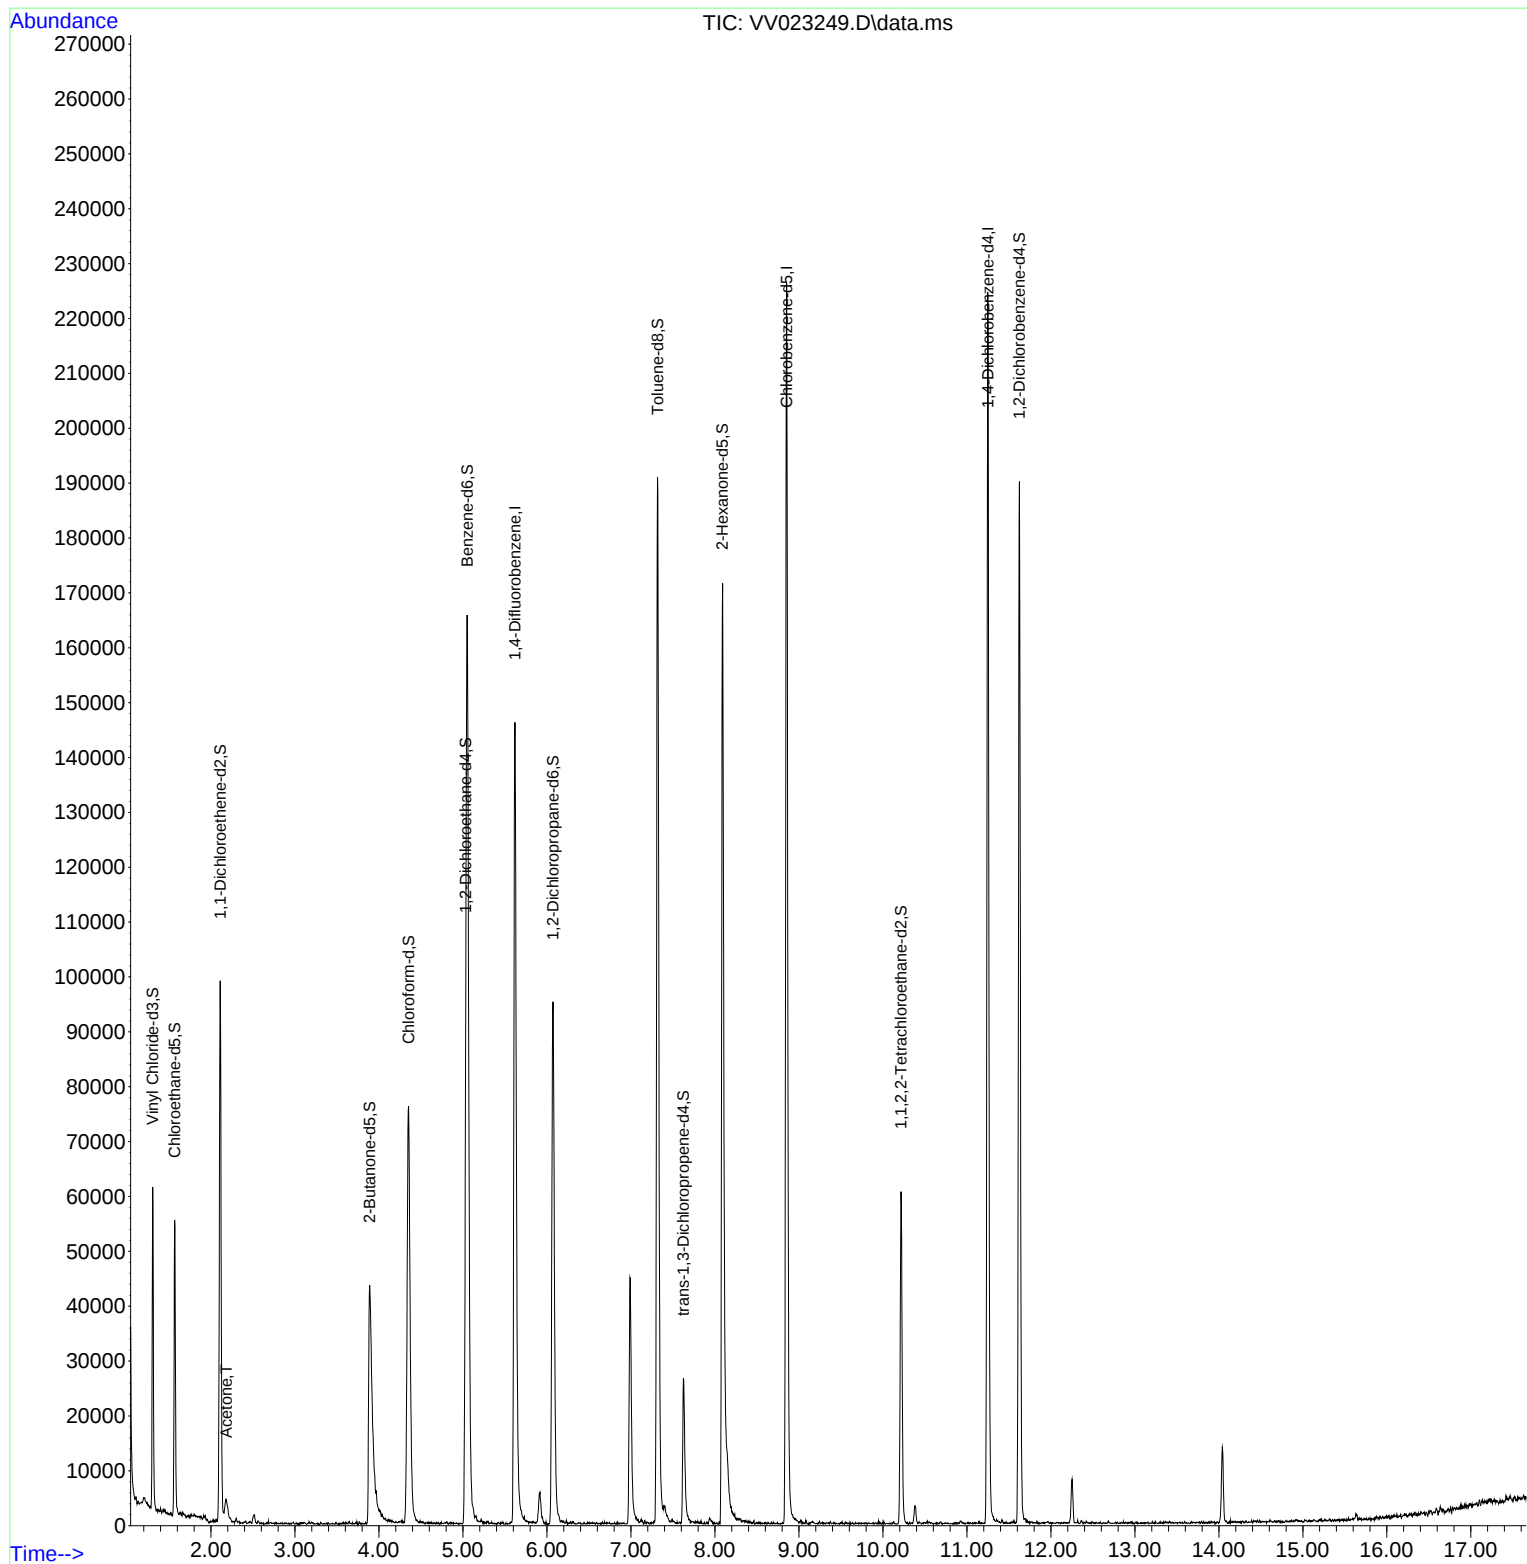

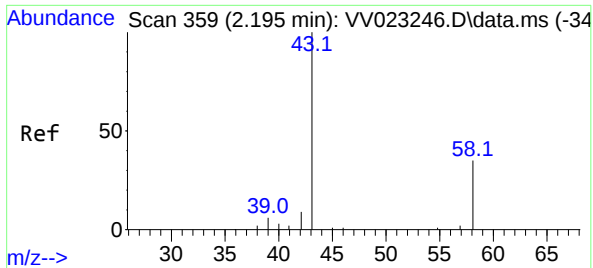

#13
Acetone
Concen: 7.409 ug/L
RT: 2.182 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV023249.D
Acq: 05 Nov 2021 22:15

Instrument :
MSVOA_V
ClientSampleId :
H4570

Tgt Ion: 43 Resp: 6352
Ion Ratio Lower Upper
43 100
58 31.2 0.0 55.4

