

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110521\
 Data File : VW023259.D
 Acq On : 06 Nov 2021 02:08
 Operator : SY/MD
 Sample : M4534-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB858

Quant Time: Nov 09 04:32:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 03:48:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	137114	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	138087	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62500	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	38287	4.457	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.200%	
7) Chloroethane-d5	1.571	69	34361	4.908	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.200%	
11) 1,1-Dichloroethene-d2	2.111	63	55765	3.468	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.400%	
20) 2-Butanone-d5	3.892	46	92084	62.225	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	124.460%	
24) Chloroform-d	4.352	84	86458	4.723	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
26) 1,2-Dichloroethane-d4	5.034	65	41363	5.025	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.400%	
32) Benzene-d6	5.053	84	163600	4.617	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	6.072	67	49960	4.790	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.800%	
41) Toluene-d8	7.317	98	141425	4.260	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.628	79	16598	4.197	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.000%	
46) 2-Hexanone-d5	8.088	63	65556	45.054	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.100%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34295	4.572	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54484	5.235	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	104.800%	
Target Compounds						Qvalue
51) Chlorobenzene	8.889	112	2925	0.107	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023259.D
Acq On : 06 Nov 2021 02:08
Operator : SY/MD
Sample : M4534-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB858

Quant Time: Nov 09 04:32:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 03:48:20 2021
Response via : Initial Calibration

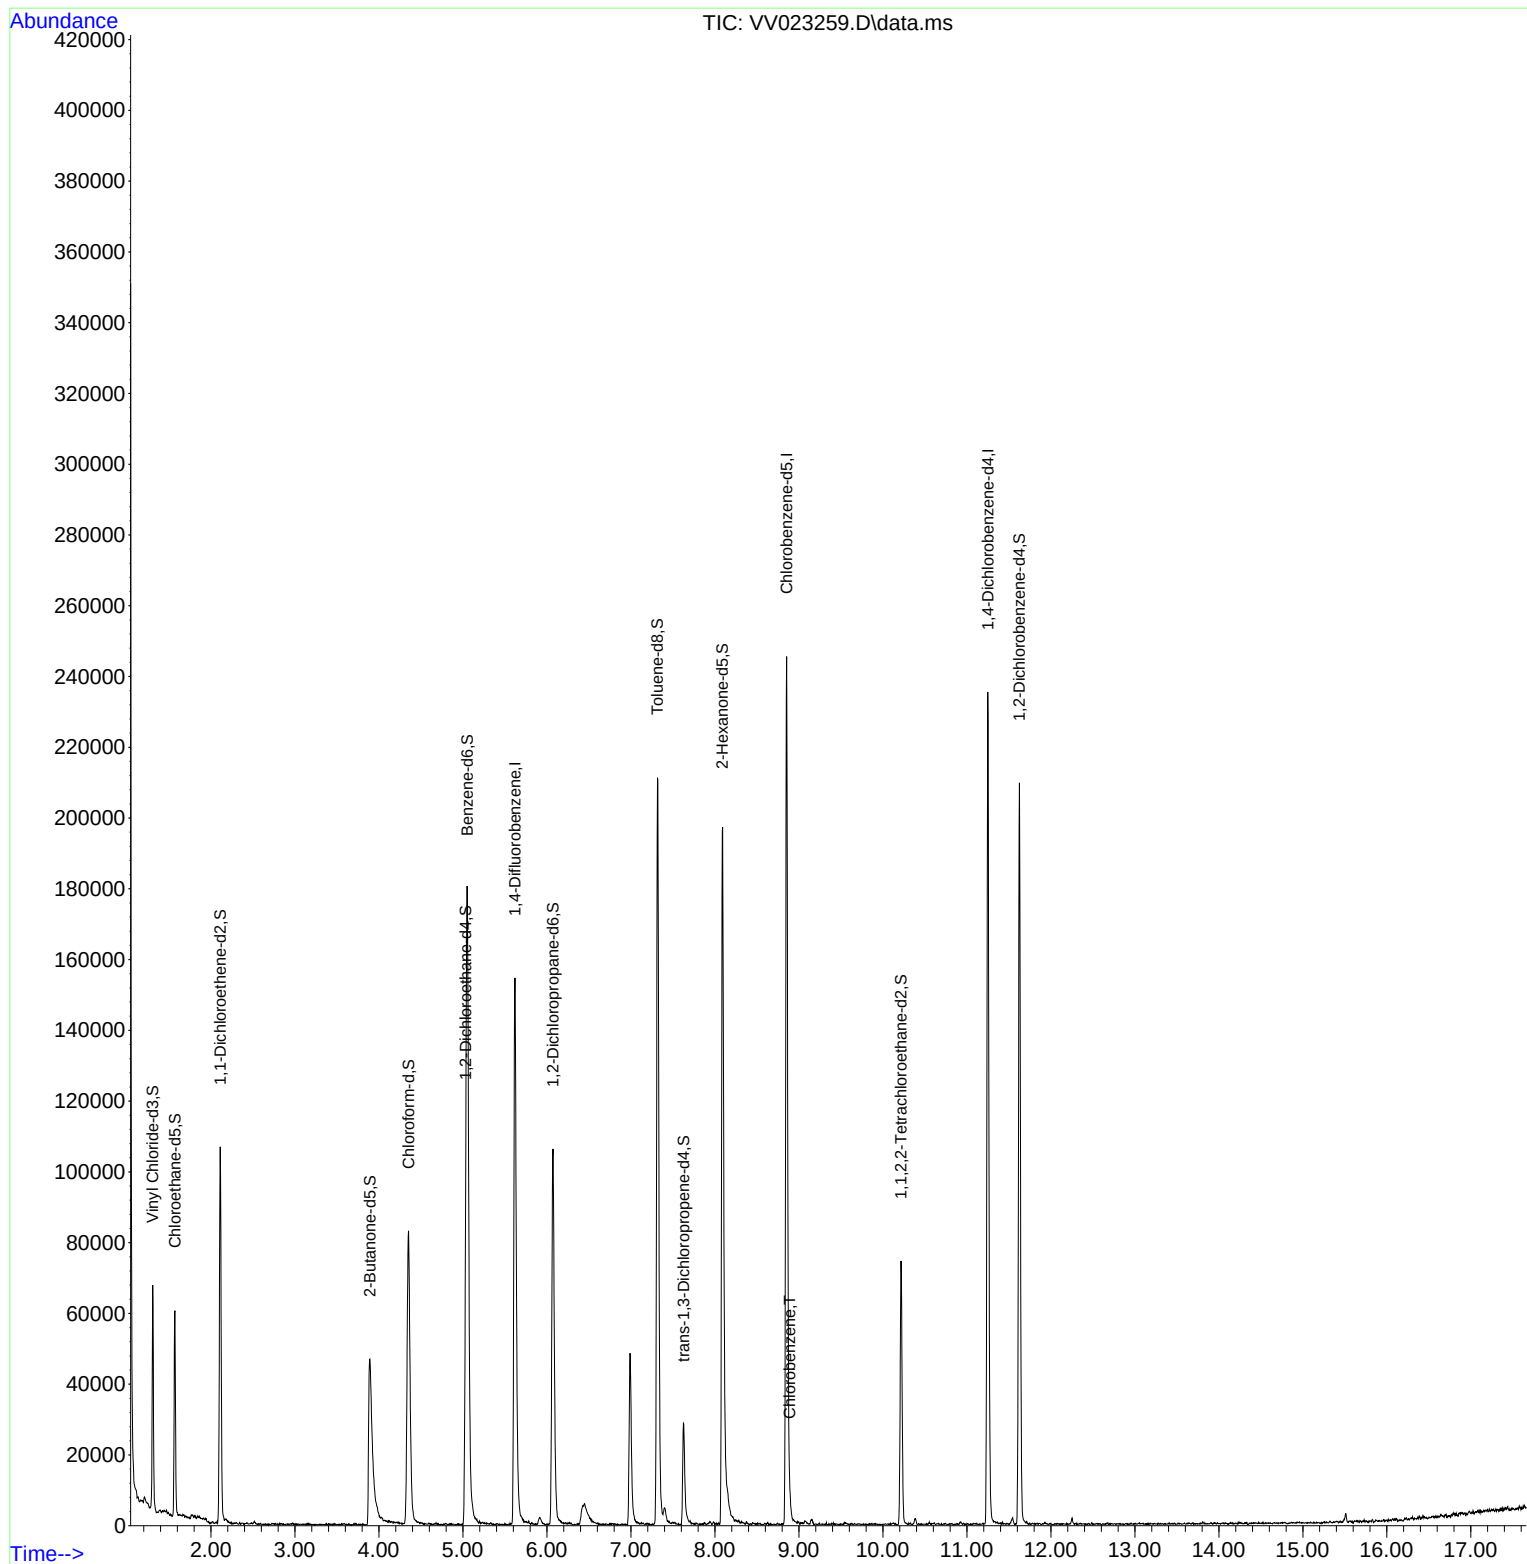

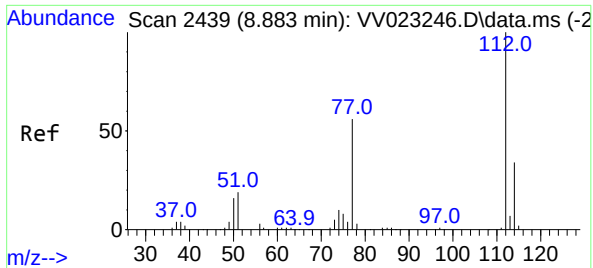

#51
 Chlorobenzene
 Concen: 0.107 ug/L
 RT: 8.889 min Scan# 24
 Delta R.T. 0.006 min
 Lab File: VV023259.D
 Acq: 06 Nov 2021 02:08

Instrument :
 MSVOA_V
 ClientSampleId :
 GB858

Tgt Ion:112 Resp: 2925

Ion	Ratio	Lower	Upper
112	100		
114	34.2	22.0	40.8
77	58.2	44.4	66.6

