

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110521\
 Data File : VW023262.D
 Acq On : 06 Nov 2021 03:17
 Operator : SY/MD
 Sample : M4534-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB859

Quant Time: Nov 09 04:37:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 09 03:48:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	142446	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	140171	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65549	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	38610	4.327	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.600%	
7) Chloroethane-d5	1.571	69	34488	4.742	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.111	63	56342	3.373	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.400%	
20) 2-Butanone-d5	3.892	46	95568	62.162	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	124.320%	
24) Chloroform-d	4.352	84	87507	4.601	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	5.034	65	41258	4.824	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
32) Benzene-d6	5.053	84	167117	4.647	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.072	67	51392	4.854	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.317	98	142462	4.227	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.600%	
43) trans-1,3-Dichloroprop...	7.625	79	17860	4.449	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.092	63	70361	47.637	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.280%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34917	4.586	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	56595	5.185	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.800%	
Target Compounds					Qvalue	
42) Toluene	7.400	91	6032	0.144	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023262.D
Acq On : 06 Nov 2021 03:17
Operator : SY/MD
Sample : M4534-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB859

Quant Time: Nov 09 04:37:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 09 03:48:20 2021
Response via : Initial Calibration

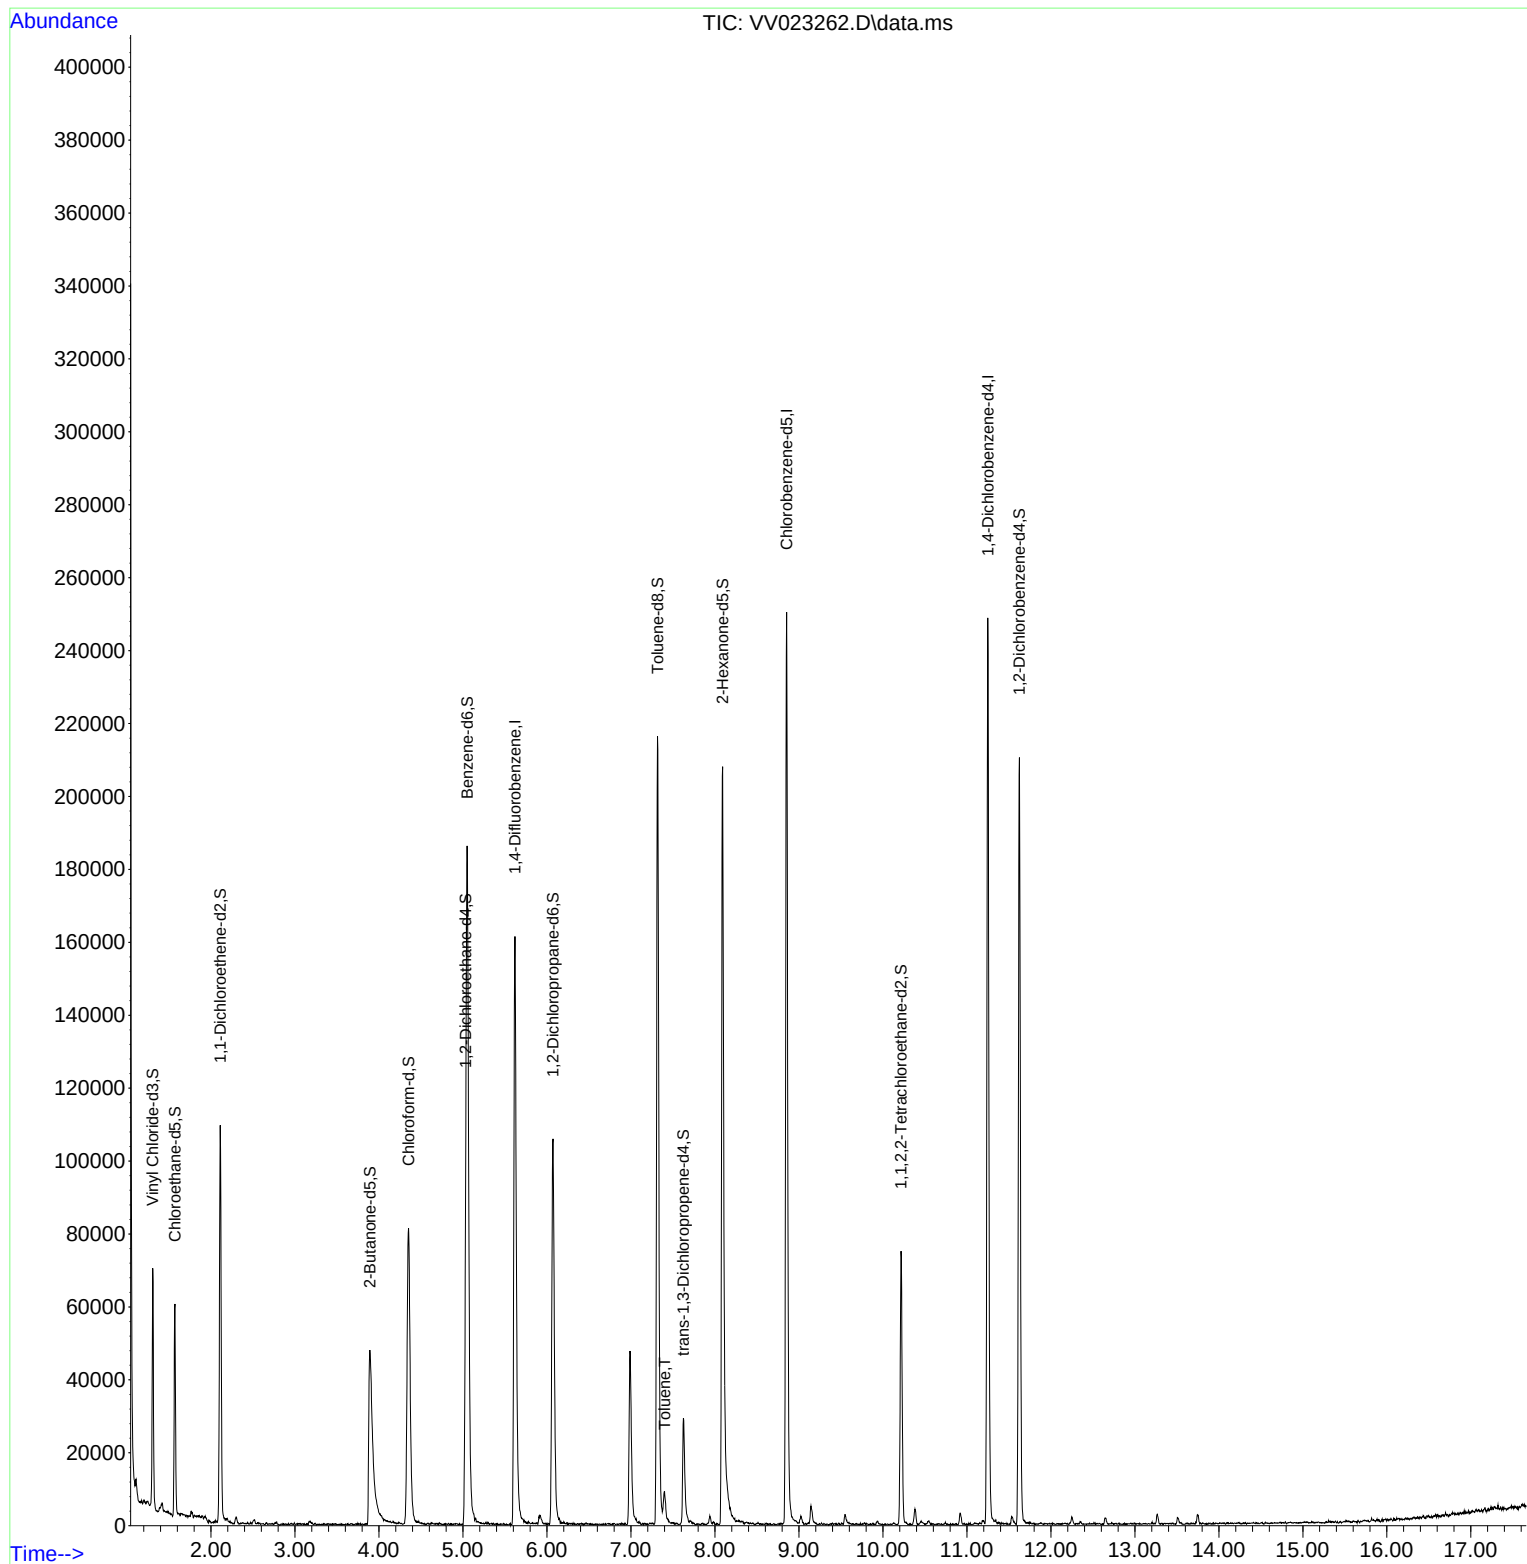

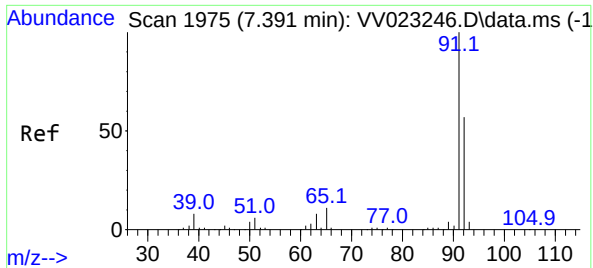

#42
Toluene
Concen: 0.144 ug/L
RT: 7.400 min Scan# 19
Delta R.T. 0.010 min
Lab File: VV023262.D
Acq: 06 Nov 2021 03:17

Instrument :
MSVOA_V
ClientSampleId :
GB859

Tgt Ion: 91 Resp: 6032
Ion Ratio Lower Upper
91 100
92 65.9 39.3 72.9

