

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023220.D
 Acq On : 05 Nov 2021 10:29
 Operator : SY/MD
 Sample : VV1105WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	91	rVB	65678	67318	15.27%	1.949%
2	1.564	155	163	172	rBV	59368	64964	14.73%	1.881%
3	2.105	319	331	348	rBV	114482	161974	36.74%	4.690%
4	2.503	444	455	467	rVB3	5036	8732	1.98%	0.253%
5	3.899	880	889	916	rBV2	26132	93875	21.29%	2.718%
6	4.346	1008	1028	1055	rBV	77662	199967	45.36%	5.790%
7	5.043	1228	1245	1271	rBV2	175440	440888	100.00%	12.765%
8	5.613	1411	1422	1445	rBV	138865	285273	64.70%	8.260%
9	5.908	1505	1514	1526	rVB7	2319	4809	1.09%	0.139%
10	6.066	1551	1563	1587	rBV	100764	207282	47.01%	6.002%
11	6.985	1838	1849	1872	rBV	45785	88574	20.09%	2.565%
12	7.313	1940	1951	1973	rBV	207366	361483	81.99%	10.466%
13	7.394	1974	1976	1990	rVB5	2938	4559	1.03%	0.132%
14	7.622	2036	2047	2072	rBV2	26808	51938	11.78%	1.504%
15	8.088	2182	2192	2224	rBV	150284	316795	71.85%	9.172%
16	8.850	2418	2429	2453	rBV	216514	353814	80.25%	10.244%
17	10.217	2843	2854	2871	rBV	66839	106635	24.19%	3.087%
18	11.249	3163	3175	3193	rBV	206745	324921	73.70%	9.408%
19	11.625	3280	3292	3314	rBV	194637	310004	70.31%	8.976%




Sum of corrected areas: 3453805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023220.D
Acq On : 05 Nov 2021 10:29
Operator : SY/MD
Sample : VV1105WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

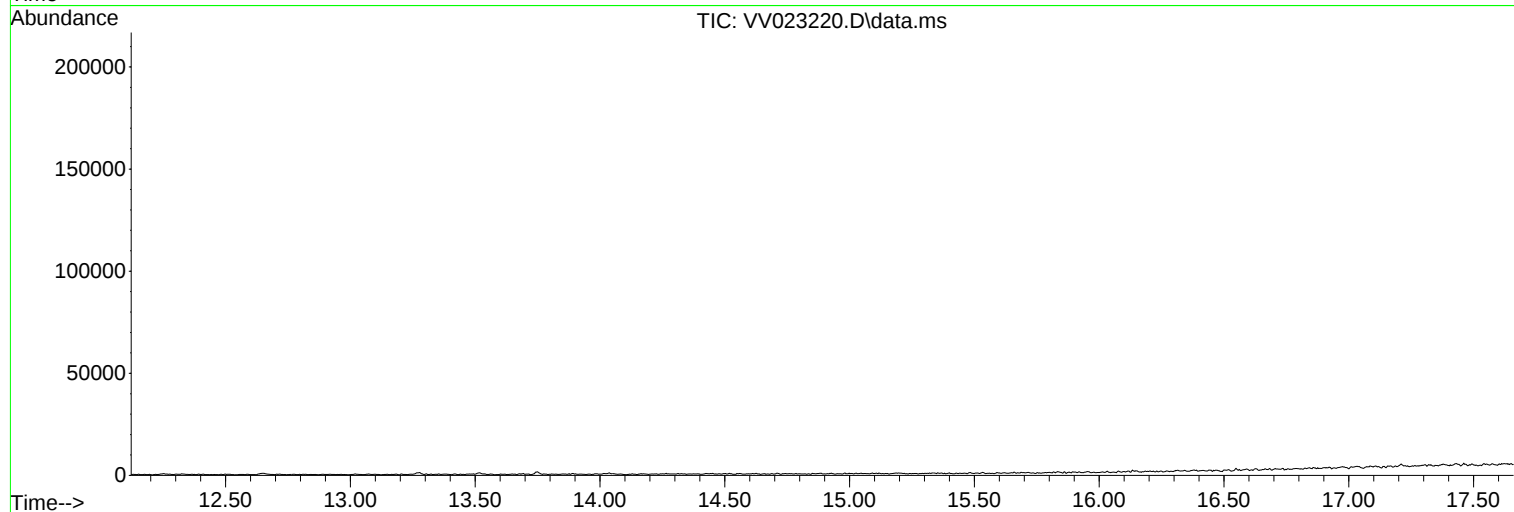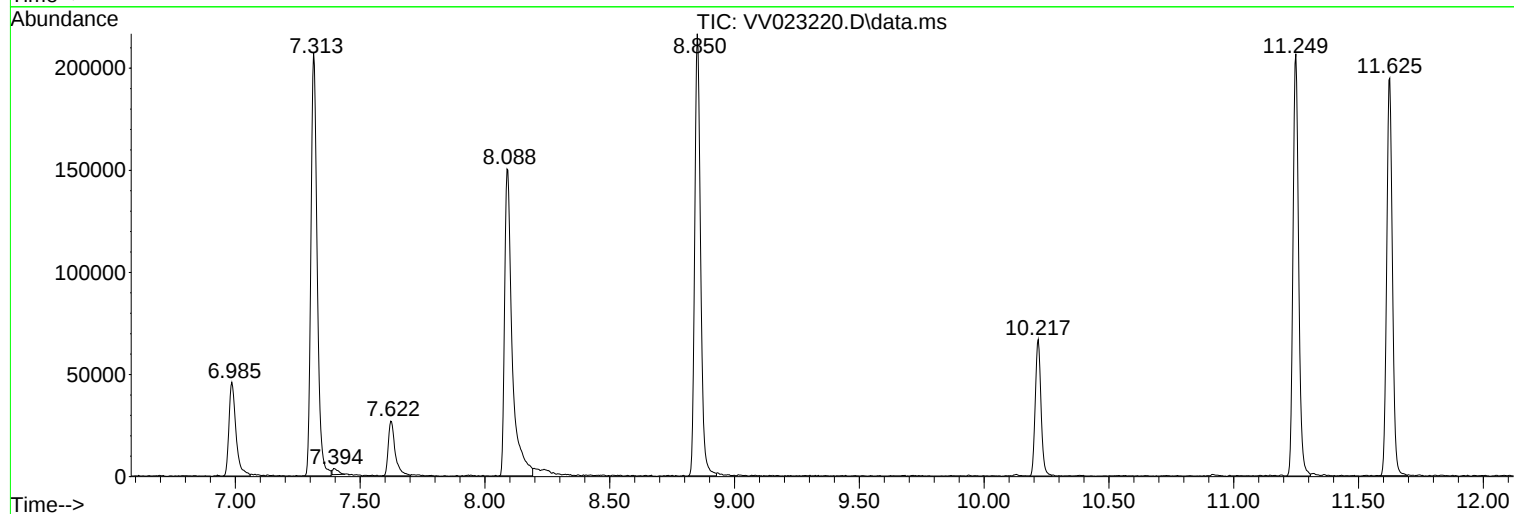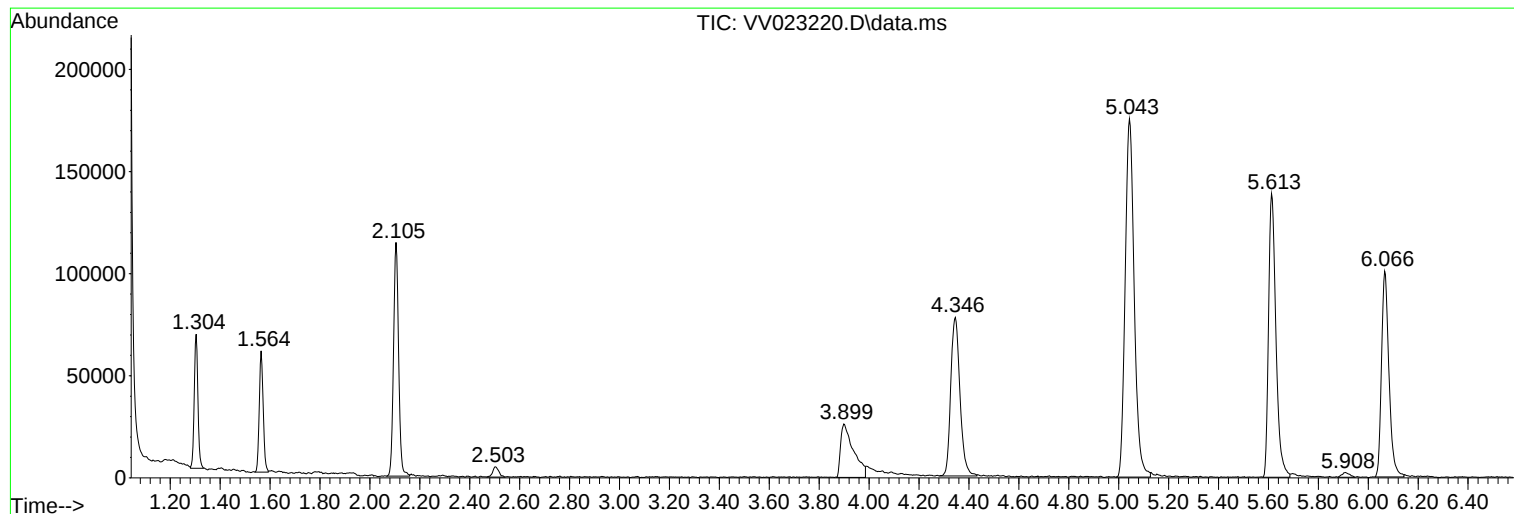

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023220.D
Acq On : 05 Nov 2021 10:29
Operator : SY/MD
Sample : VV1105WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023220.D
Acq On : 05 Nov 2021 10:29
Operator : SY/MD
Sample : VV1105WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc