

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023222.D
 Acq On : 05 Nov 2021 11:16
 Operator : SY/MD
 Sample : M4492-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	73	rVB2	5051	5908	1.24%	0.154%
2	1.307	76	83	95	rVB	69882	72498	15.19%	1.890%
3	1.568	156	164	176	rBV	58083	67552	14.15%	1.761%
4	2.108	321	332	349	rBV	113487	164337	34.43%	4.284%
5	3.912	882	893	931	rBV2	31586	130219	27.28%	3.394%
6	4.352	1013	1030	1055	rBV	85380	218164	45.71%	5.687%
7	5.050	1231	1247	1271	rBV2	191848	477303	100.00%	12.442%
8	5.619	1412	1424	1445	rBV	149917	305689	64.05%	7.969%
9	5.921	1506	1518	1537	rBV4	15961	35247	7.38%	0.919%
10	6.072	1551	1565	1586	rBV	108654	226890	47.54%	5.914%
11	6.992	1839	1851	1867	rBV	48190	91978	19.27%	2.398%
12	7.317	1940	1952	1972	rBV	221524	393486	82.44%	10.257%
13	7.625	2038	2048	2073	rBV	28588	54788	11.48%	1.428%
14	8.091	2183	2193	2227	rBV2	174747	367075	76.91%	9.569%
15	8.853	2419	2430	2454	rBV	234082	386909	81.06%	10.086%
16	10.217	2840	2854	2874	rBV	74007	121424	25.44%	3.165%
17	11.249	3165	3175	3196	rBV	223264	350729	73.48%	9.143%
18	11.532	3253	3263	3276	rBV2	10777	19146	4.01%	0.499%
19	11.625	3280	3292	3315	rVB	220580	346841	72.67%	9.041%




Sum of corrected areas: 3836183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023222.D
Acq On : 05 Nov 2021 11:16
Operator : SY/MD
Sample : M4492-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

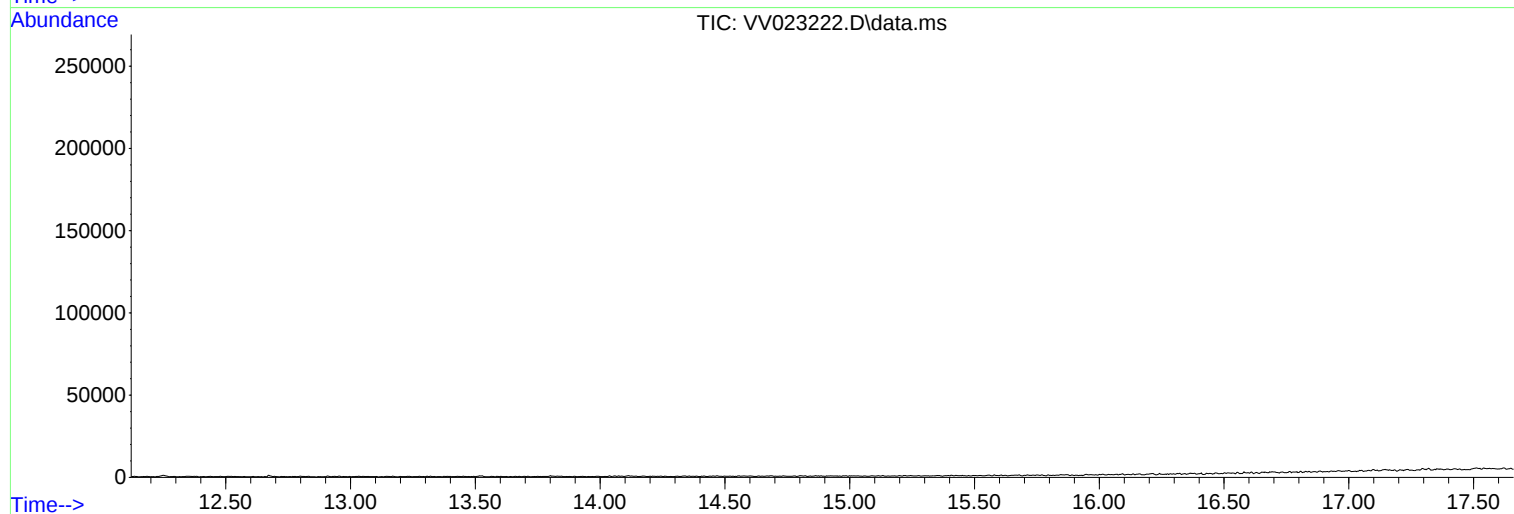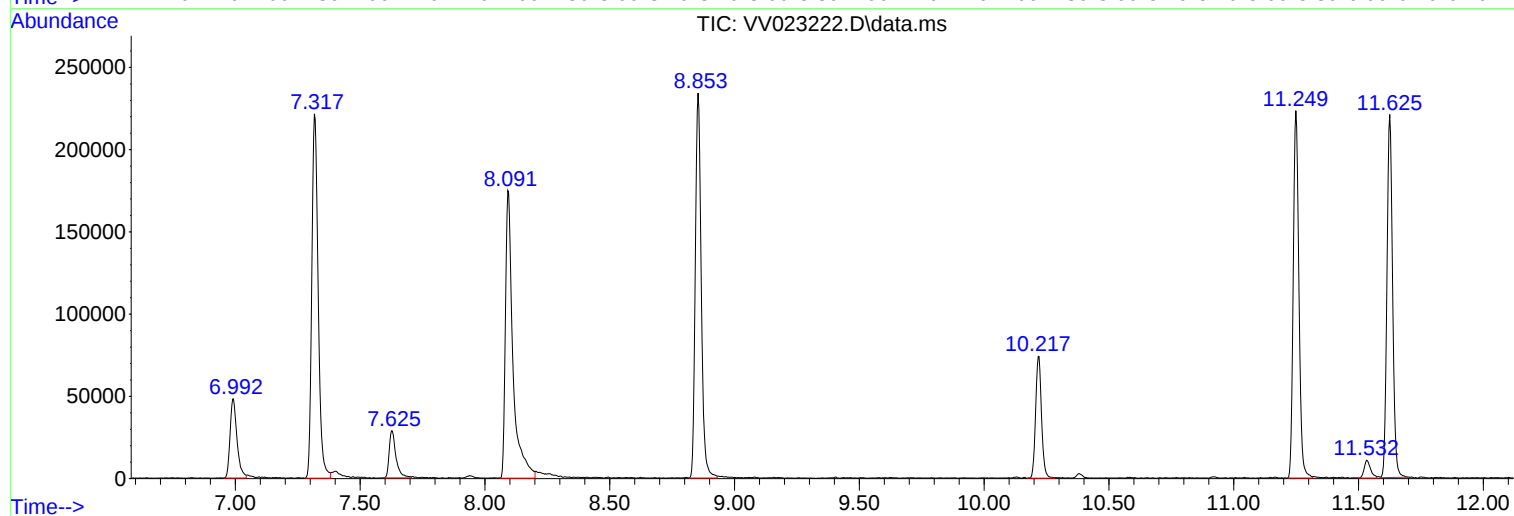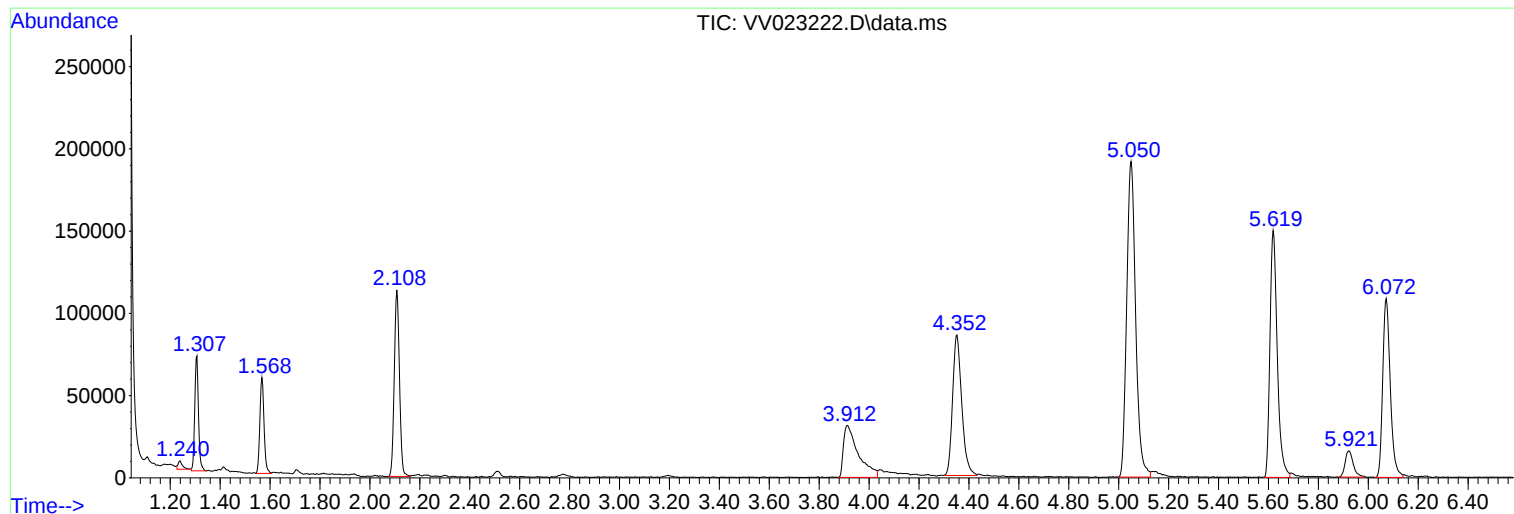

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023222.D
Acq On : 05 Nov 2021 11:16
Operator : SY/MD
Sample : M4492-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023222.D
Acq On : 05 Nov 2021 11:16
Operator : SY/MD
Sample : M4492-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc