

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023226.D
 Acq On : 05 Nov 2021 12:53
 Operator : SY/MD
 Sample : M4492-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	67687	68933	14.79%	1.868%
2	1.568	156	164	176	rVB	59163	66738	14.32%	1.808%
3	2.108	318	332	347	rBV	111020	161081	34.55%	4.364%
4	3.912	881	893	922	rBV2	27688	106693	22.89%	2.891%
5	4.352	1013	1030	1055	rBV	81802	208389	44.70%	5.646%
6	5.050	1231	1247	1276	rBV2	186603	466205	100.00%	12.632%
7	5.619	1412	1424	1451	rBV	148030	302664	64.92%	8.201%
8	5.921	1507	1518	1530	rBV8	6866	15231	3.27%	0.413%
9	6.072	1551	1565	1585	rBV2	104685	218511	46.87%	5.920%
10	6.989	1840	1850	1871	rBV	45496	89810	19.26%	2.433%
11	7.317	1940	1952	1971	rBV	217704	378863	81.27%	10.265%
12	7.397	1971	1977	1992	rVB4	4024	8616	1.85%	0.233%
13	7.625	2039	2048	2065	rBV2	28397	51107	10.96%	1.385%
14	8.092	2183	2193	2231	rBV	169527	360719	77.37%	9.774%
15	8.854	2417	2430	2458	rBV	229524	378241	81.13%	10.248%
16	10.217	2840	2854	2873	rBV	76267	119380	25.61%	3.235%
17	11.249	3164	3175	3193	rBV	219103	340689	73.08%	9.231%
18	11.535	3253	3264	3279	rBV4	8064	15502	3.33%	0.420%
19	11.625	3279	3292	3311	rVV	217405	333385	71.51%	9.033%




Sum of corrected areas: 3690757

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023226.D
Acq On : 05 Nov 2021 12:53
Operator : SY/MD
Sample : M4492-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

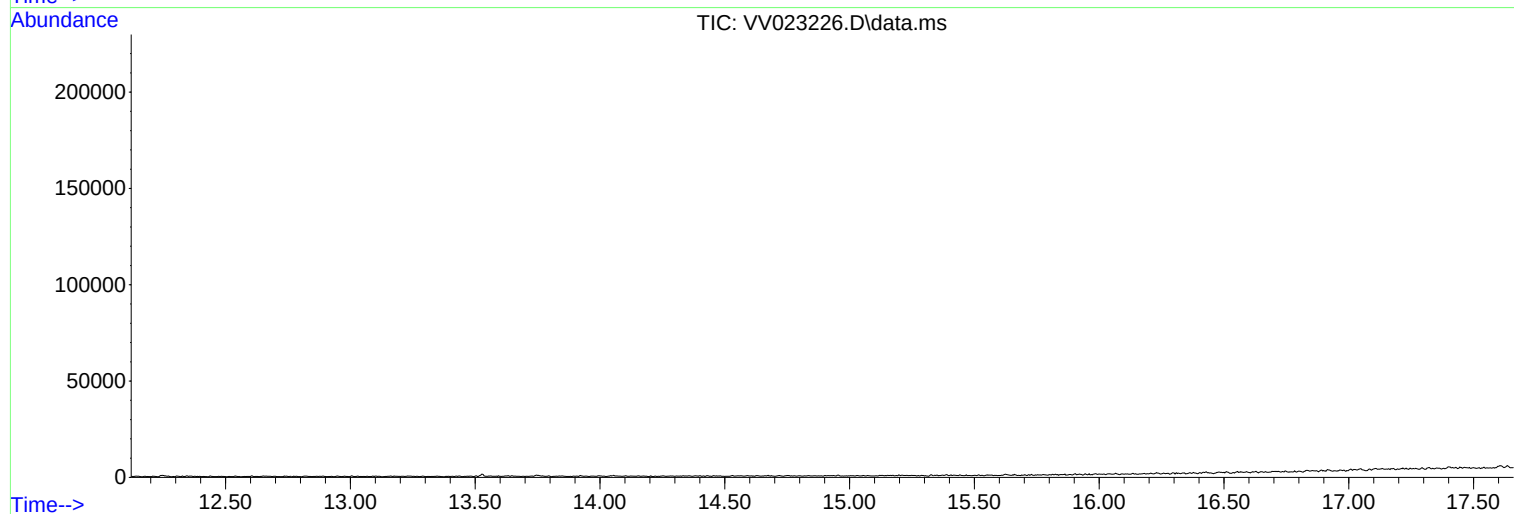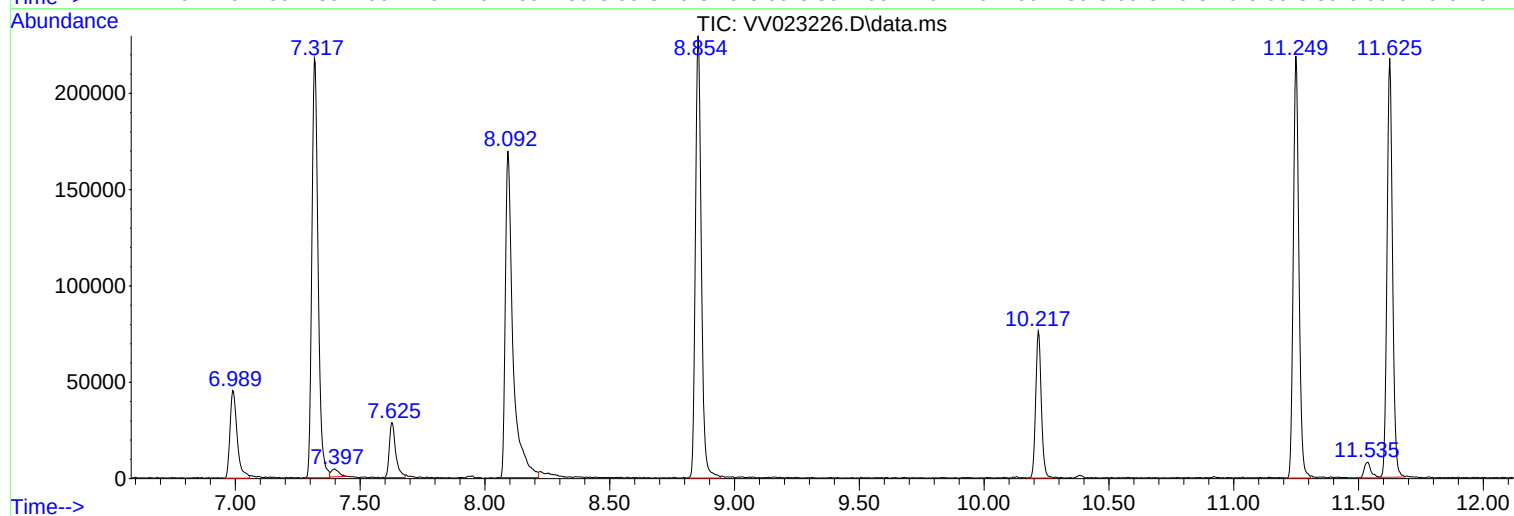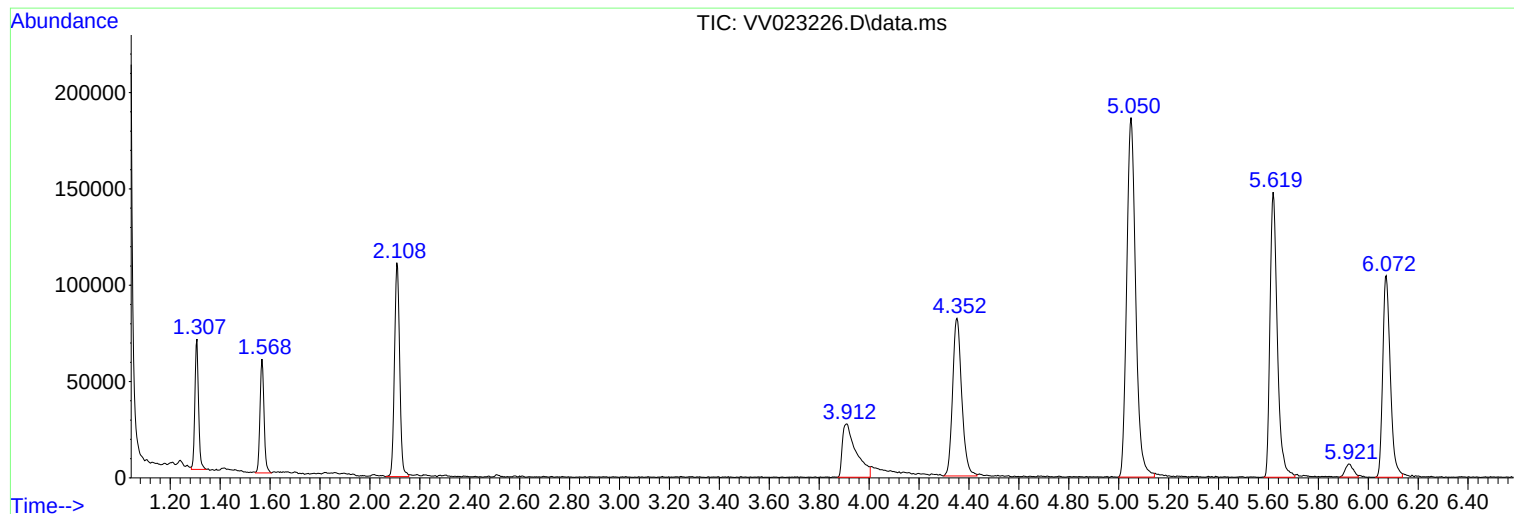

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023226.D
Acq On : 05 Nov 2021 12:53
Operator : SY/MD
Sample : M4492-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023226.D
Acq On : 05 Nov 2021 12:53
Operator : SY/MD
Sample : M4492-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
