

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023227.D
 Acq On : 05 Nov 2021 13:17
 Operator : SY/MD
 Sample : M4492-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.236	59	61	72	rVB2	4613	5356	1.08%	0.136%
2	1.307	76	83	95	rVB	66889	70281	14.14%	1.786%
3	1.567	156	164	177	rBV	60119	66592	13.40%	1.692%
4	2.108	321	332	348	rBV	112743	163101	32.82%	4.145%
5	3.908	882	892	924	rBV2	30247	122172	24.58%	3.105%
6	4.352	1011	1030	1060	rBV2	84557	212897	42.84%	5.411%
7	5.050	1231	1247	1280	rBV2	192302	496938	100.00%	12.630%
8	5.619	1409	1424	1454	rBV	139790	290216	58.40%	7.376%
9	5.918	1505	1517	1538	rBV	78848	163590	32.92%	4.158%
10	6.072	1552	1565	1586	rBV	108046	224342	45.14%	5.702%
11	6.988	1839	1850	1874	rBV2	48460	94199	18.96%	2.394%
12	7.316	1941	1952	1974	rBV	223104	396376	79.76%	10.074%
13	7.625	2035	2048	2074	rBV	29290	56885	11.45%	1.446%
14	8.091	2183	2193	2224	rBV	175967	374995	75.46%	9.531%
15	8.853	2419	2430	2455	rBV	220230	364974	73.44%	9.276%
16	10.217	2844	2854	2873	rBV	75088	120768	24.30%	3.069%
17	11.249	3165	3175	3192	rBV	217278	335350	67.48%	8.523%
18	11.535	3250	3264	3279	rBV3	13521	25612	5.15%	0.651%
19	11.625	3281	3292	3308	rBV	222132	349903	70.41%	8.893%




Sum of corrected areas: 3934547

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023227.D
Acq On : 05 Nov 2021 13:17
Operator : SY/MD
Sample : M4492-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

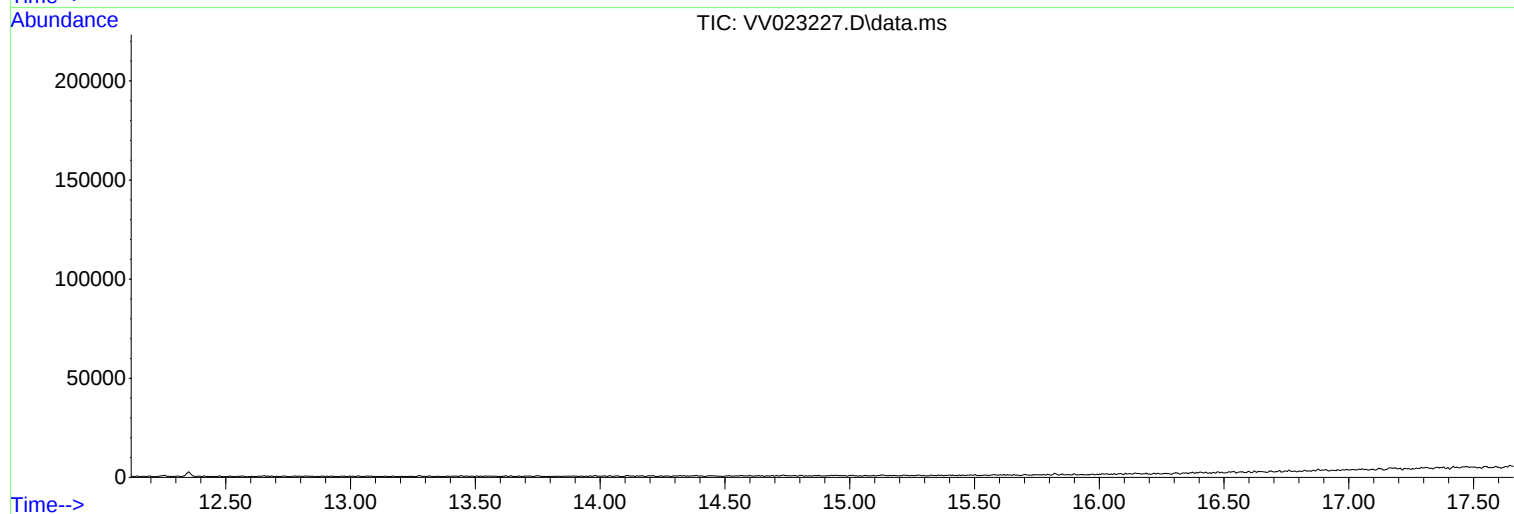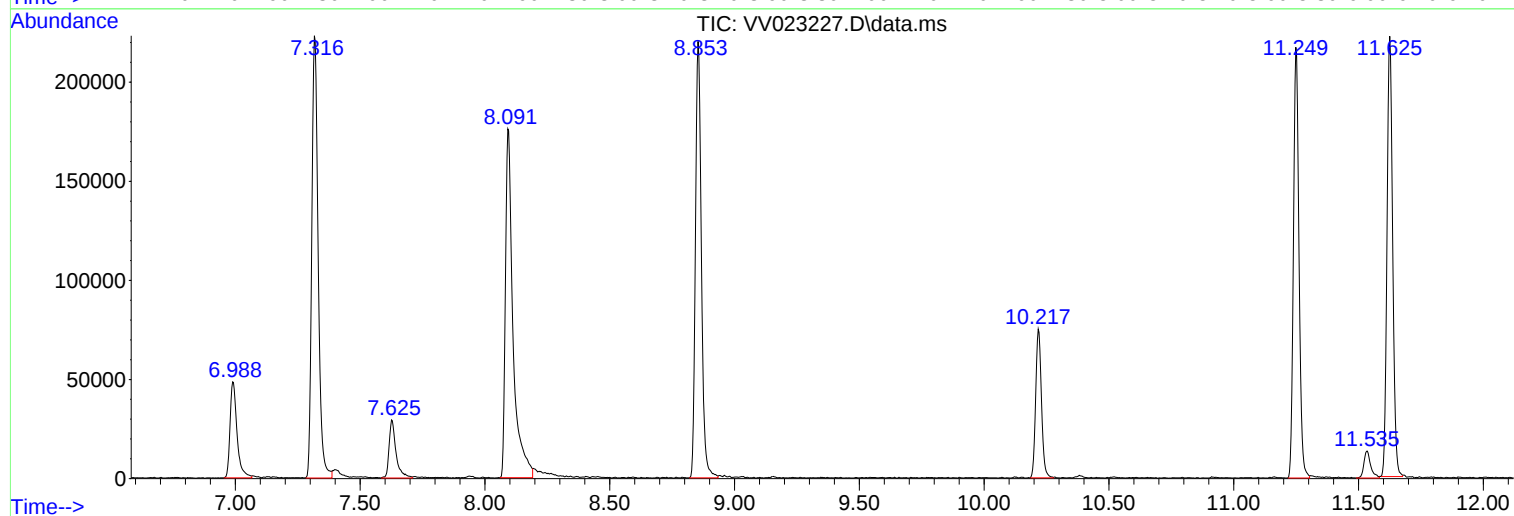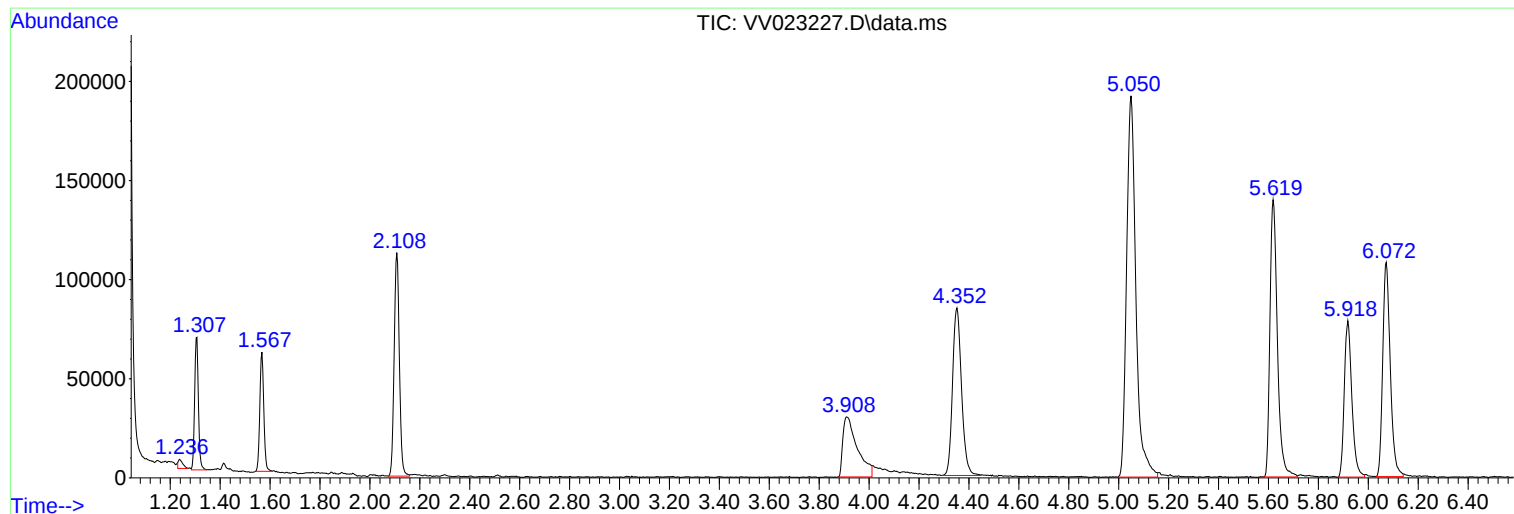

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023227.D
Acq On : 05 Nov 2021 13:17
Operator : SY/MD
Sample : M4492-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023227.D
Acq On : 05 Nov 2021 13:17
Operator : SY/MD
Sample : M4492-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
