

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023229.D
 Acq On : 05 Nov 2021 14:03
 Operator : SY/MD
 Sample : M4492-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	76	rVB3	6235	8313	1.89%	0.247%
2	1.304	76	82	98	rVB	65018	66934	15.23%	1.990%
3	1.417	112	117	124	rVB2	3646	4579	1.04%	0.136%
4	1.568	157	164	176	rBV	55582	62198	14.15%	1.850%
5	2.108	321	332	347	rBV	109066	154303	35.11%	4.588%
6	3.905	879	891	892	rBV	28321	35747	8.13%	1.063%
7	4.352	1014	1030	1053	rBV2	77323	196331	44.67%	5.838%
8	5.050	1228	1247	1272	rBV4	177302	439527	100.00%	13.070%
9	5.619	1410	1424	1452	rBV	131306	269217	61.25%	8.006%
10	6.072	1552	1565	1588	rBV	100817	208296	47.39%	6.194%
11	6.989	1839	1850	1870	rBV2	44024	83841	19.08%	2.493%
12	7.317	1937	1952	1973	rBV	203396	359293	81.75%	10.684%
13	7.397	1973	1977	1989	rVB4	2560	4446	1.01%	0.132%
14	7.629	2038	2049	2072	rBV	27484	52241	11.89%	1.553%
15	8.092	2183	2193	2221	rBV	156236	324768	73.89%	9.658%
16	8.854	2419	2430	2456	rBV	206214	339353	77.21%	10.091%
17	10.217	2841	2854	2872	rBV	68944	110409	25.12%	3.283%
18	11.249	3161	3175	3191	rBV	194790	304839	69.36%	9.065%
19	11.532	3253	3263	3274	rBV3	13457	24260	5.52%	0.721%
20	11.625	3281	3292	3308	rBV	199311	313947	71.43%	9.336%




Sum of corrected areas: 3362842

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023229.D
Acq On : 05 Nov 2021 14:03
Operator : SY/MD
Sample : M4492-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

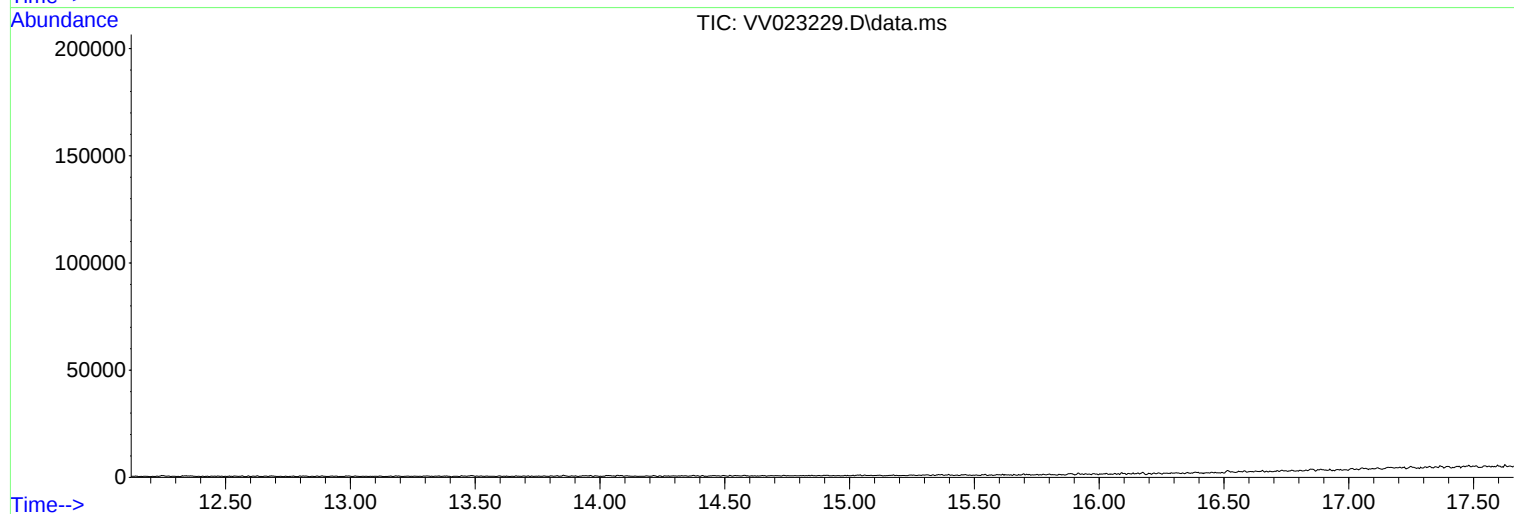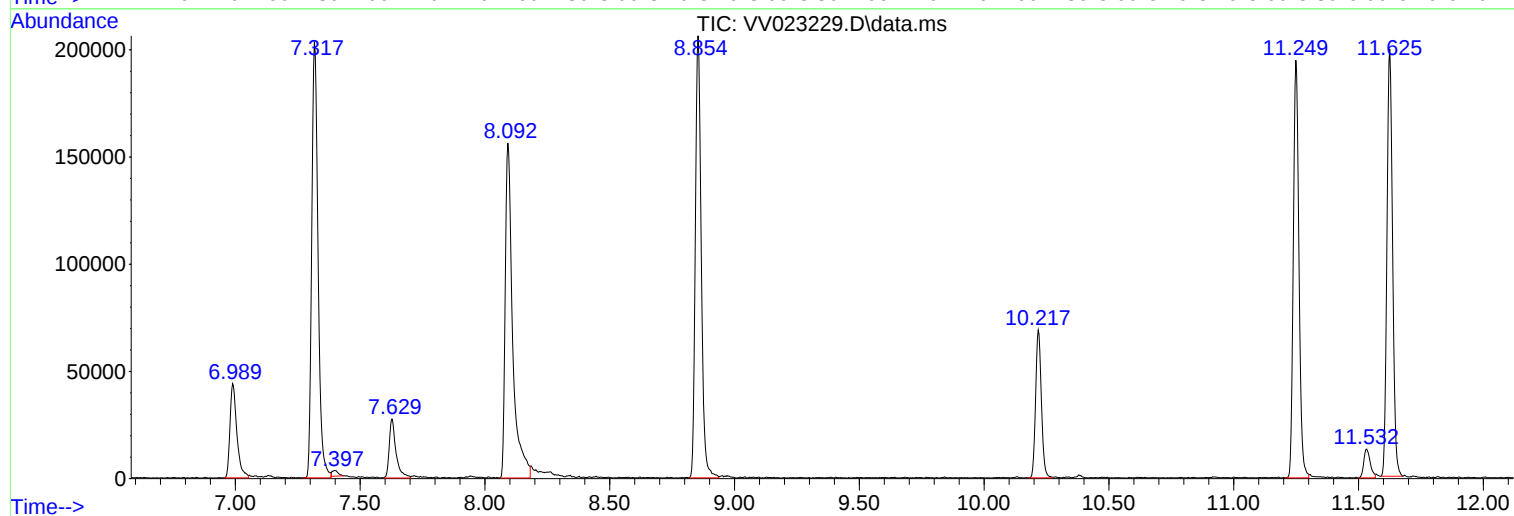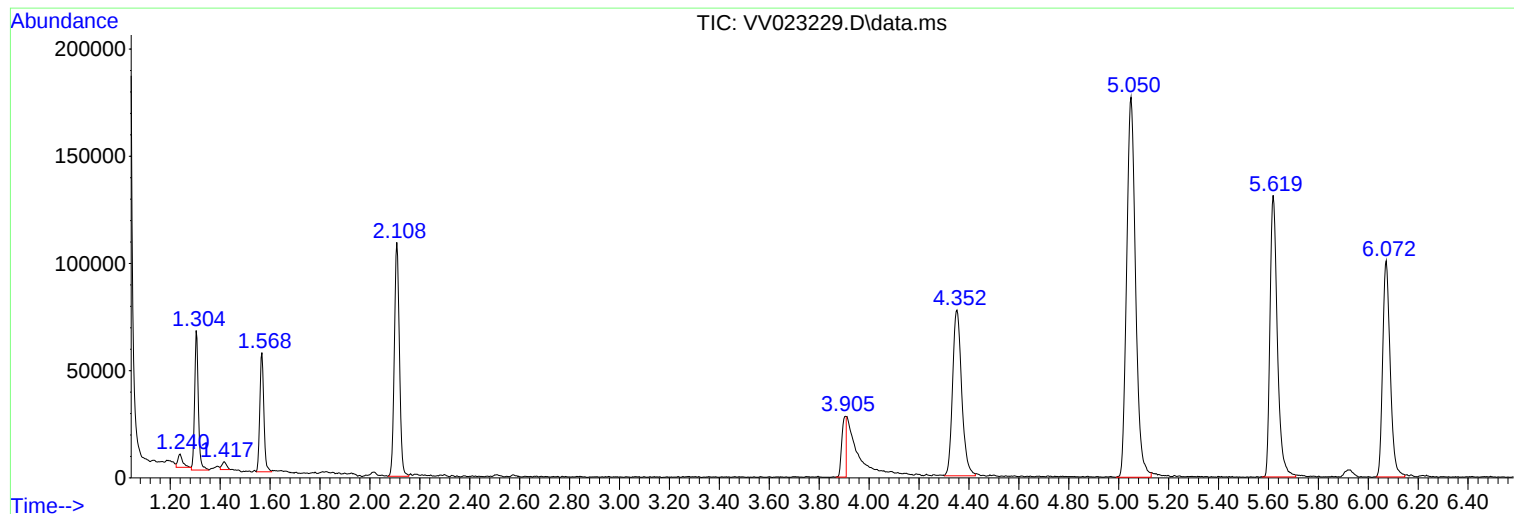

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023229.D
Acq On : 05 Nov 2021 14:03
Operator : SY/MD
Sample : M4492-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023229.D
Acq On : 05 Nov 2021 14:03
Operator : SY/MD
Sample : M4492-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
