

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023230.D
 Acq On : 05 Nov 2021 14:27
 Operator : SY/MD
 Sample : M4492-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1S7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	67236	67738	14.25%	1.814%
2	1.568	155	164	177	rBV	58257	66310	13.95%	1.776%
3	2.108	321	332	345	rBV	116328	162747	34.24%	4.358%
4	2.577	465	478	491	rVB2	19937	35510	7.47%	0.951%
5	3.909	883	892	922	rBV2	26515	106856	22.48%	2.861%
6	4.352	1015	1030	1056	rVB	83361	209815	44.14%	5.618%
7	5.050	1231	1247	1275	rBV2	190004	475372	100.00%	12.729%
8	5.619	1413	1424	1449	rBV2	141432	289544	60.91%	7.753%
9	5.912	1506	1515	1517	rBV5	4968	6264	1.32%	0.168%
10	6.072	1552	1565	1591	rBV	107112	226573	47.66%	6.067%
11	6.989	1840	1850	1880	rBV2	47887	92780	19.52%	2.484%
12	7.317	1938	1952	1971	rBV	219598	387486	81.51%	10.376%
13	7.400	1972	1978	1999	rVB5	5010	10747	2.26%	0.288%
14	7.625	2038	2048	2064	rBV2	27634	52501	11.04%	1.406%
15	8.095	2183	2194	2239	rBV2	163873	366618	77.12%	9.817%
16	8.854	2418	2430	2449	rBV	224131	372230	78.30%	9.967%
17	10.217	2842	2854	2869	rBV	69522	112903	23.75%	3.023%
18	11.249	3164	3175	3193	rBV	217748	337606	71.02%	9.040%
19	11.535	3257	3264	3274	rBV4	4028	6966	1.47%	0.187%
20	11.625	3281	3292	3308	rBV	215670	342487	72.05%	9.171%
21	12.349	3509	3517	3526	rBV4	3833	5450	1.15%	0.146%




Sum of corrected areas: 3734503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023230.D
Acq On : 05 Nov 2021 14:27
Operator : SY/MD
Sample : M4492-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

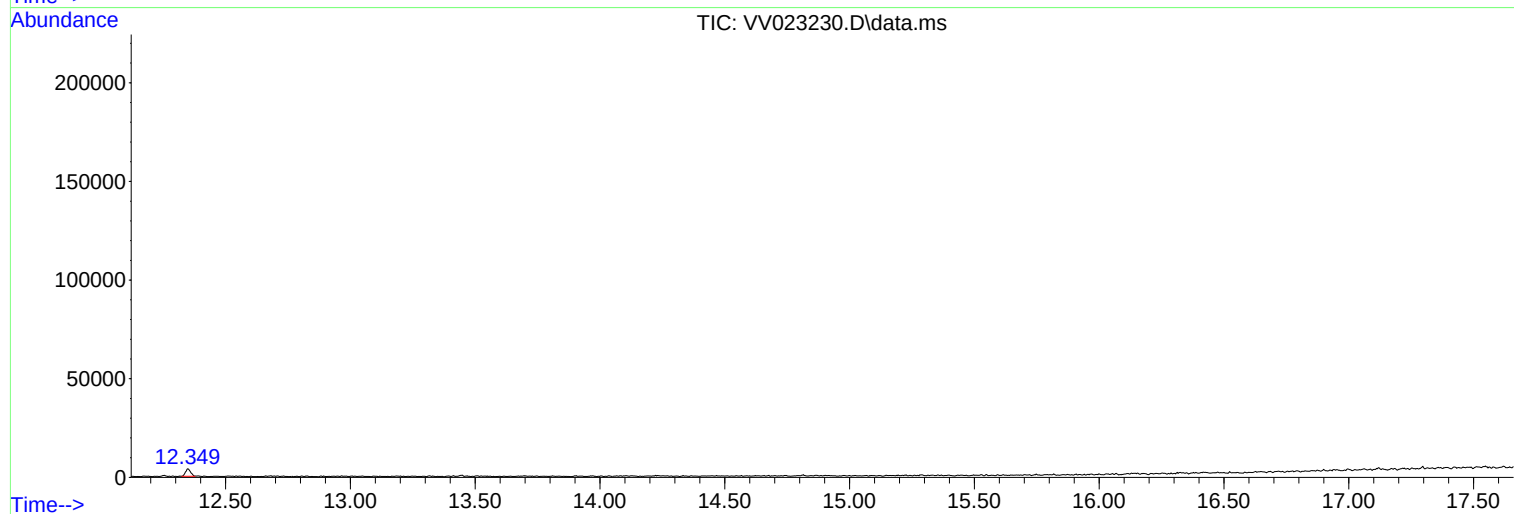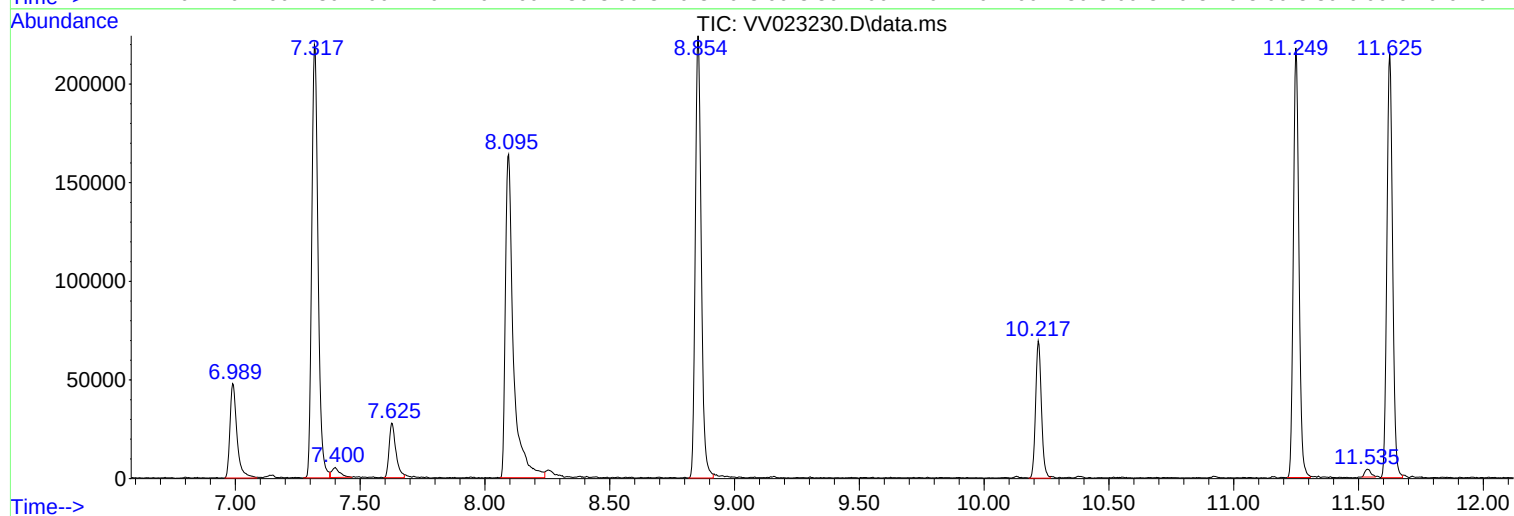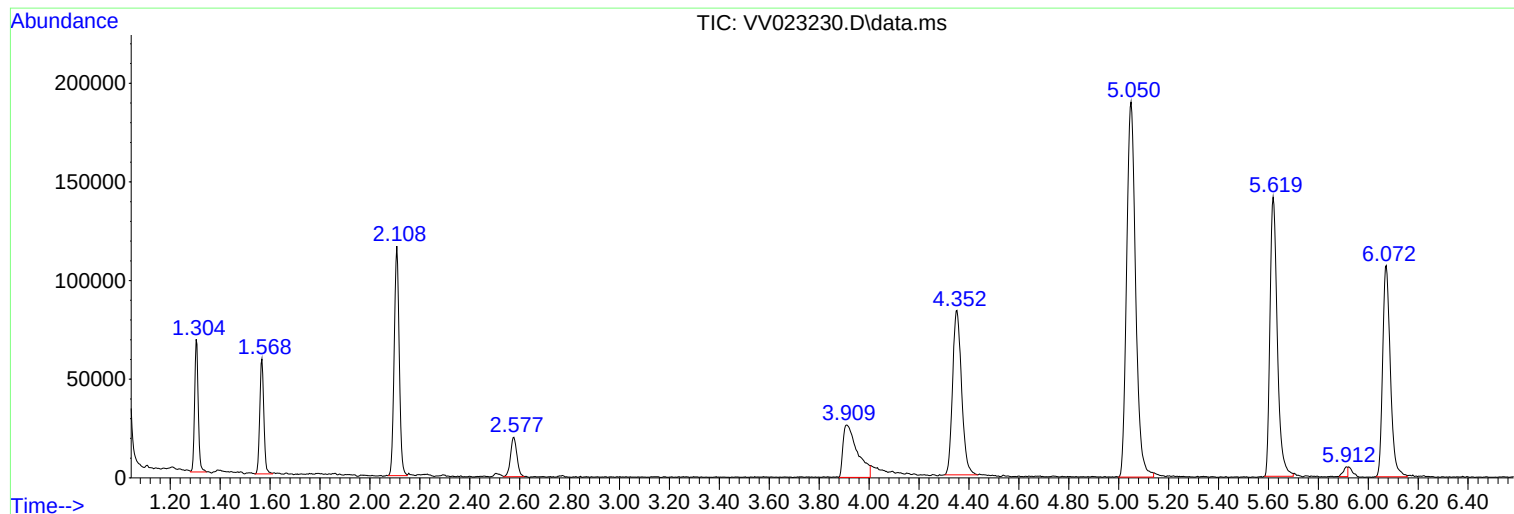

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023230.D
Acq On : 05 Nov 2021 14:27
Operator : SY/MD
Sample : M4492-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic2.577 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.577	0.61 ug/L	35510	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclobutane, methyl-	70	C5H10	000598-61-8	80
2			Cyclobutane, methyl-	70	C5H10	000598-61-8	80
3			1-Pentene	70	C5H10	000109-67-1	72
4			Cyclopentane	70	C5H10	000287-92-3	64
5			Cyclopentane	70	C5H10	000287-92-3	59

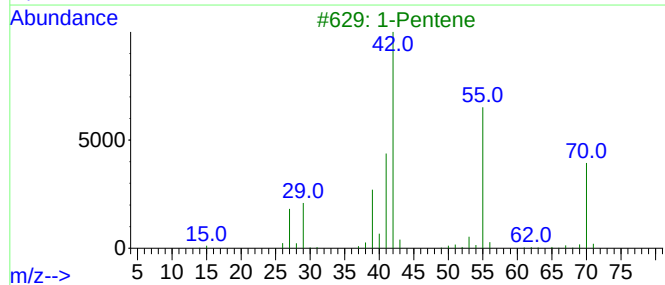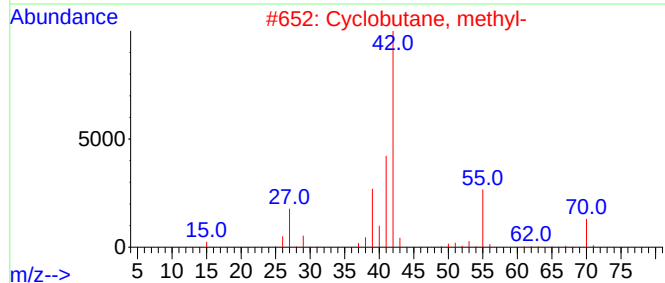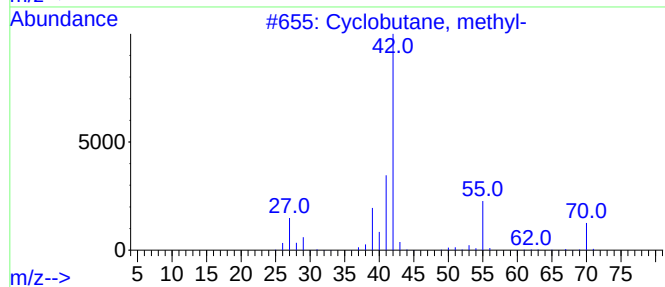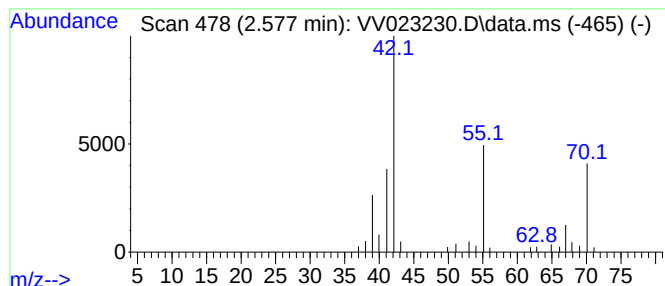

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023230.D
Acq On : 05 Nov 2021 14:27
Operator : SY/MD
Sample : M4492-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1S7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	2.577	0.6	ug/L	35510	1	5.619	289544	5.0