

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023232.D
 Acq On : 05 Nov 2021 15:13
 Operator : SY/MD
 Sample : M4464-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB7L5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	71	79	95	rVB2	90084	140508	31.25%	3.788%
2	1.568	156	164	174	rBV	55242	62061	13.80%	1.673%
3	2.108	320	332	347	rBV	103309	150471	33.47%	4.057%
4	3.908	880	892	916	rBV2	30543	112664	25.06%	3.037%
5	4.349	1011	1029	1058	rBV2	84261	214730	47.76%	5.789%
6	5.050	1232	1247	1272	rBV3	181434	449567	100.00%	12.121%
7	5.619	1412	1424	1449	rBV	145152	298951	66.50%	8.060%
8	5.915	1505	1516	1534	rVB7	6343	14383	3.20%	0.388%
9	6.072	1553	1565	1598	rBV	103517	214528	47.72%	5.784%
10	6.989	1840	1850	1877	rBV2	46716	91740	20.41%	2.473%
11	7.317	1941	1952	1970	rBV	203086	362900	80.72%	9.784%
12	7.400	1972	1978	1991	rVB3	5543	10291	2.29%	0.277%
13	7.628	2036	2049	2069	rBV2	28378	52963	11.78%	1.428%
14	8.091	2183	2193	2233	rBV2	163026	358386	79.72%	9.662%
15	8.854	2419	2430	2449	rBV	225195	374089	83.21%	10.086%
16	9.146	2511	2521	2530	rBV3	5715	9088	2.02%	0.245%
17	10.217	2842	2854	2870	rBV	66553	106708	23.74%	2.877%
18	11.249	3164	3175	3203	rBV	224599	351657	78.22%	9.481%
19	11.625	3278	3292	3312	rBV	204994	321875	71.60%	8.678%
20	15.114	4369	4377	4386	rVB7	8056	11549	2.57%	0.311%




Sum of corrected areas: 3709109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023232.D
Acq On : 05 Nov 2021 15:13
Operator : SY/MD
Sample : M4464-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

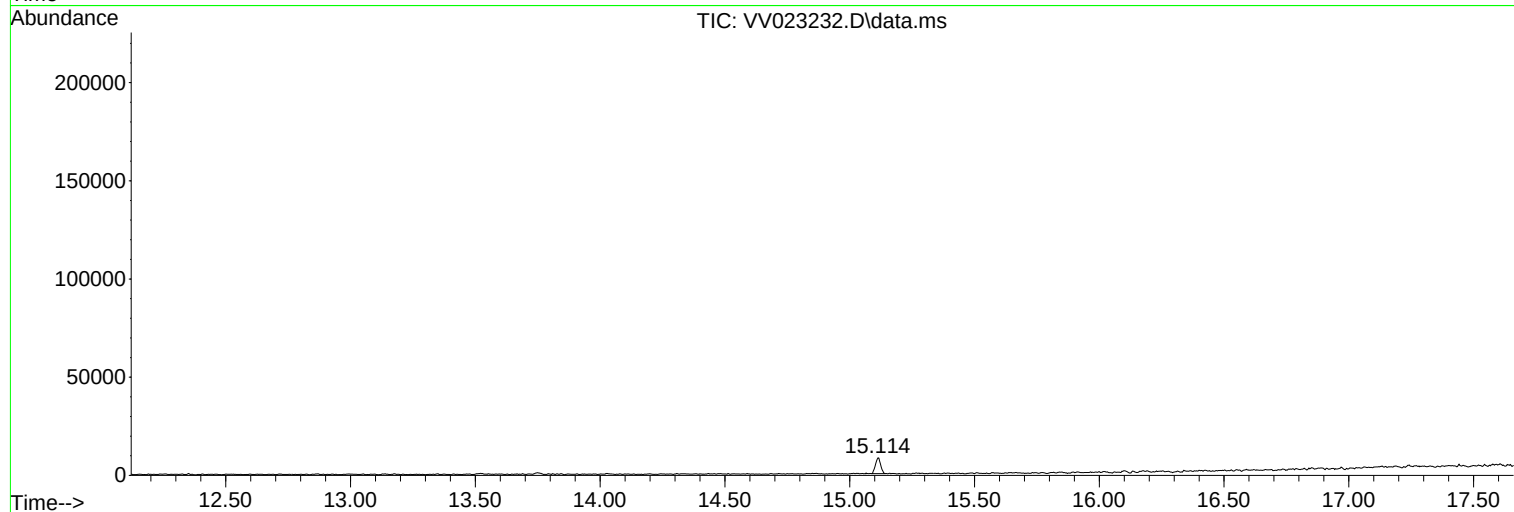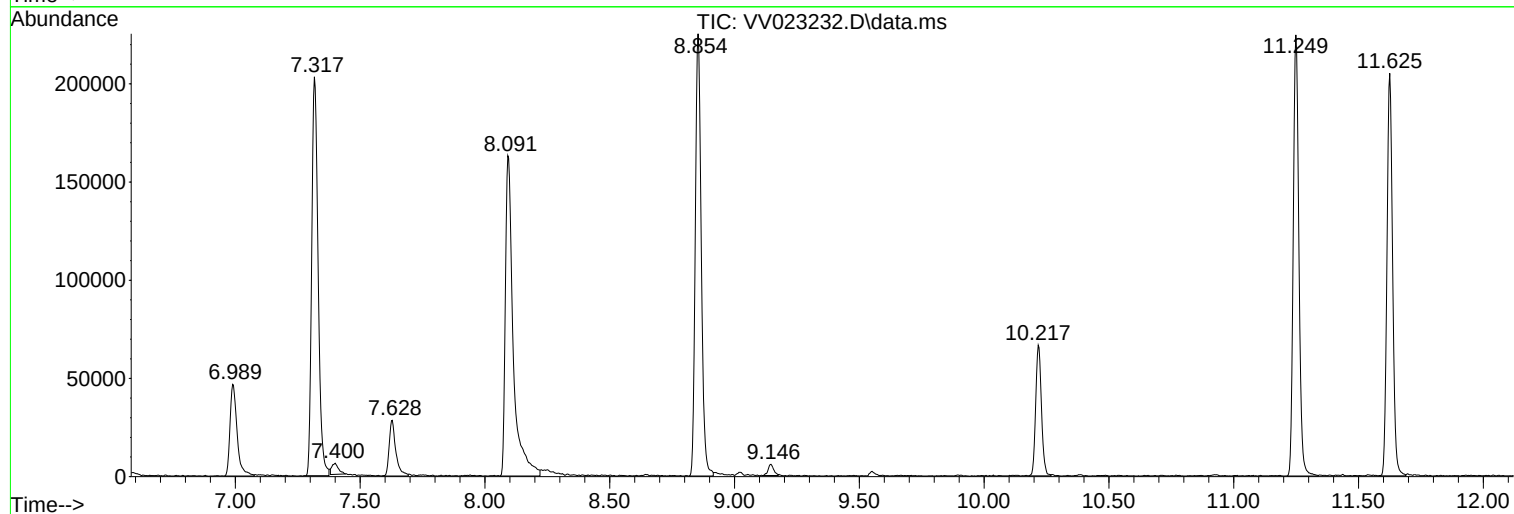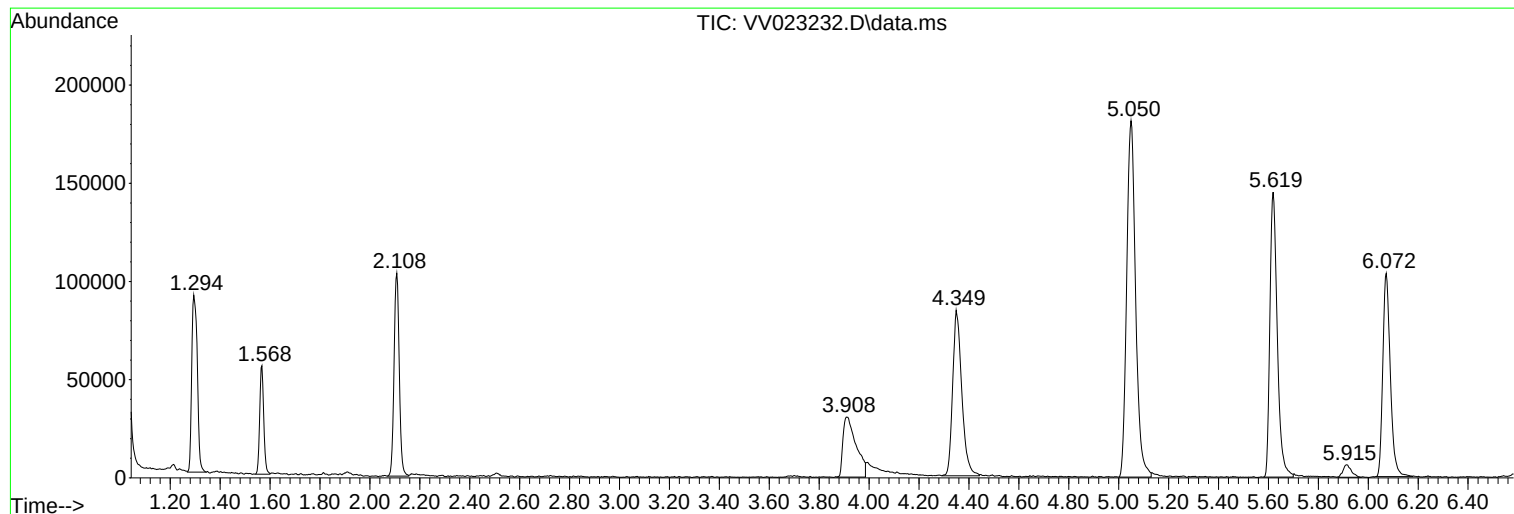

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023232.D
Acq On : 05 Nov 2021 15:13
Operator : SY/MD
Sample : M4464-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023232.D
Acq On : 05 Nov 2021 15:13
Operator : SY/MD
Sample : M4464-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB7L5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc