

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023236.D
 Acq On : 05 Nov 2021 16:47
 Operator : SY/MD
 Sample : M4535-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4620

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	41	rVB	97445	97422	12.27%	2.091%
2	1.304	75	82	94	rVB	67208	64947	8.18%	1.394%
3	1.564	156	163	176	rBV	55127	63265	7.97%	1.358%
4	2.105	320	331	345	rBV	110241	161805	20.39%	3.473%
5	2.770	521	538	552	rBV2	33398	71447	9.00%	1.533%
6	3.905	879	891	922	rBV	34310	129651	16.33%	2.783%
7	4.349	1012	1029	1057	rBV	80523	206133	25.97%	4.424%
8	5.050	1230	1247	1270	rBV2	181152	452390	57.00%	9.710%
9	5.619	1412	1424	1449	rBV	143601	294741	37.13%	6.326%
10	5.918	1505	1517	1533	rBV3	40761	84622	10.66%	1.816%
11	6.072	1550	1565	1590	rBV	102260	214927	27.08%	4.613%
12	6.989	1840	1850	1871	rBV	45493	85768	10.81%	1.841%
13	7.317	1941	1952	1973	rBV	204902	369334	46.53%	7.927%
14	7.625	2038	2048	2066	rBV	27268	50472	6.36%	1.083%
15	7.976	2144	2157	2180	rBV	471068	793724	100.00%	17.036%
16	8.091	2183	2193	2230	rVV	179730	372660	46.95%	7.998%
17	8.854	2419	2430	2450	rBV	228649	374038	47.12%	8.028%
18	10.217	2843	2854	2871	rBV	74267	114505	14.43%	2.458%
19	11.249	3164	3175	3194	rBV	216441	336938	42.45%	7.232%
20	11.625	3279	3292	3308	rBV	203372	320358	40.36%	6.876%




Sum of corrected areas: 4659147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023236.D
Acq On : 05 Nov 2021 16:47
Operator : SY/MD
Sample : M4535-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

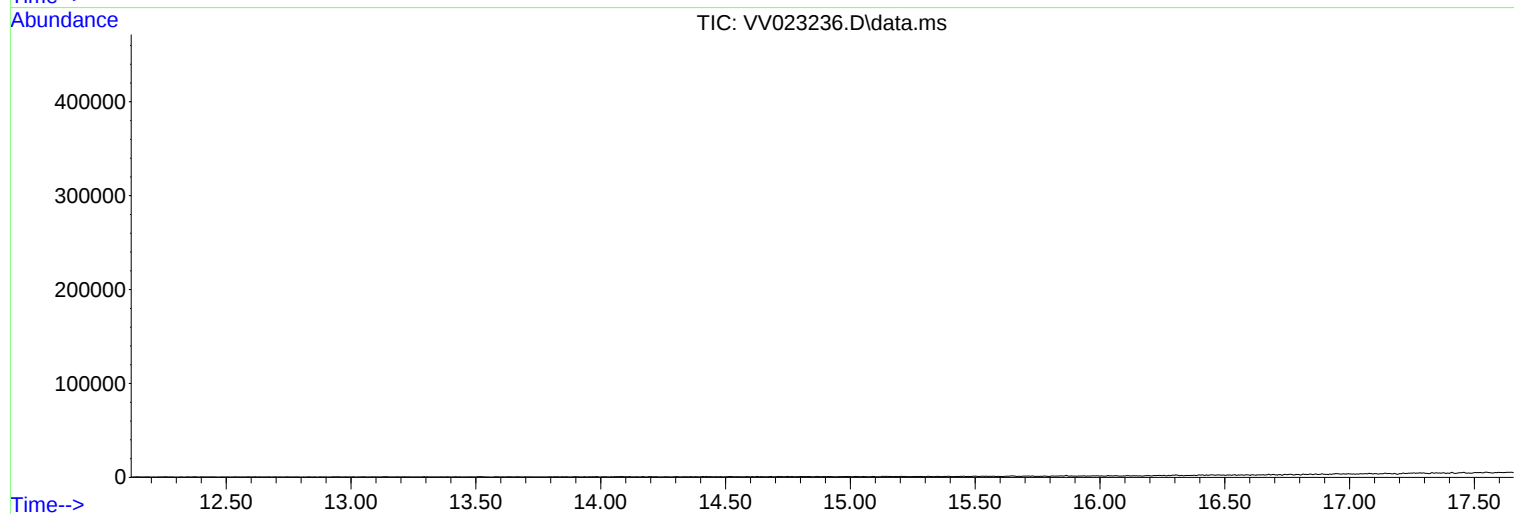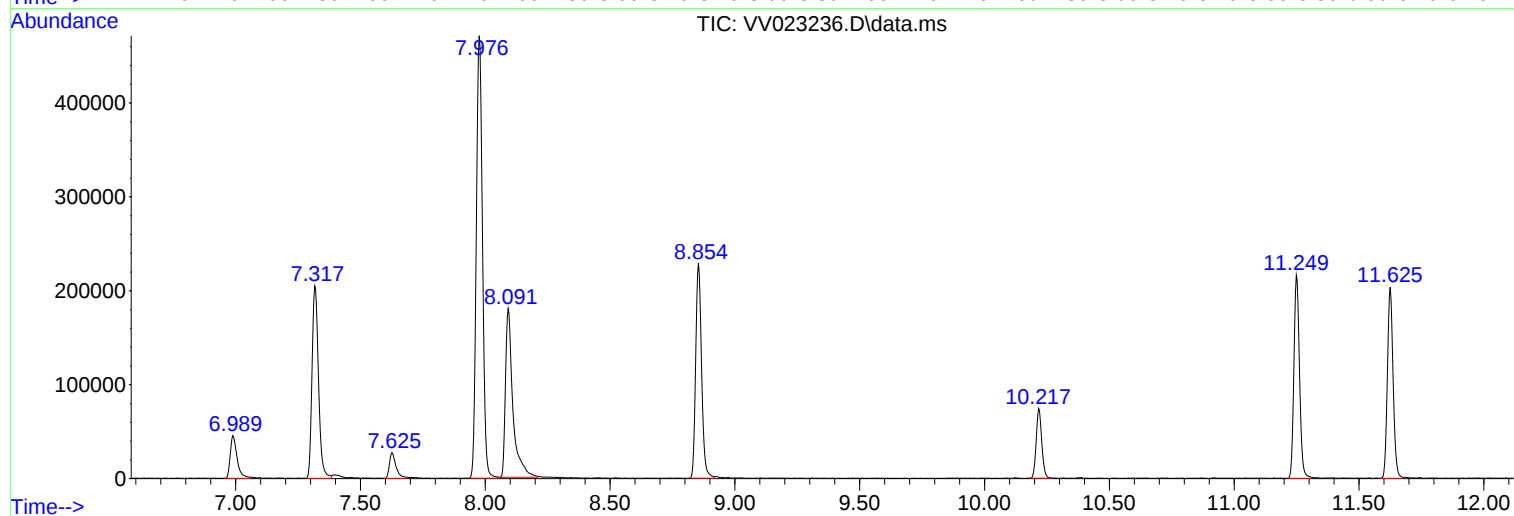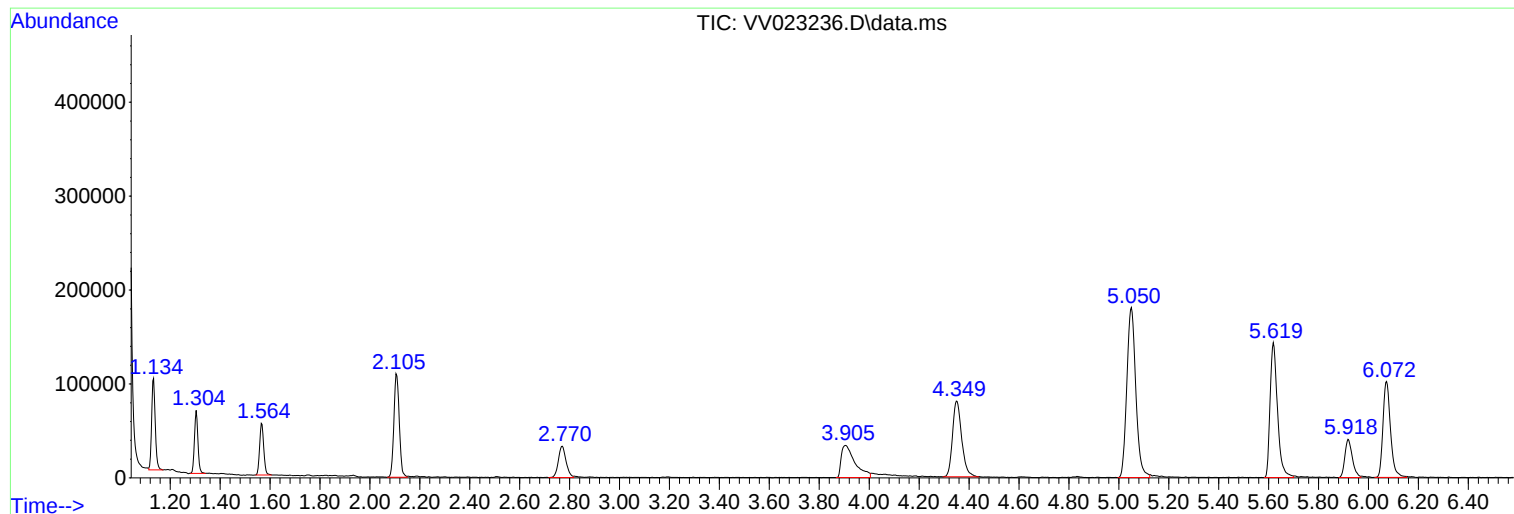

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023236.D
Acq On : 05 Nov 2021 16:47
Operator : SY/MD
Sample : M4535-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023236.D
Acq On : 05 Nov 2021 16:47
Operator : SY/MD
Sample : M4535-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
