

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023237.D
 Acq On : 05 Nov 2021 17:10
 Operator : SY/MD
 Sample : M4535-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4621

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	22	28	42	rVB	94256	97050	21.61%	2.657%
2	1.304	75	82	91	rVB	63567	62685	13.96%	1.716%
3	1.564	156	163	172	rBV	54692	60009	13.36%	1.643%
4	2.105	321	331	345	rBV	109323	154883	34.49%	4.241%
5	2.767	525	537	549	rBV3	4077	8930	1.99%	0.245%
6	3.905	881	891	927	rBV	29119	114070	25.41%	3.123%
7	4.349	1013	1029	1056	rBV2	83906	210663	46.92%	5.768%
8	5.047	1228	1246	1275	rBV2	179166	449004	100.00%	12.294%
9	5.619	1412	1424	1446	rBV	141731	290951	64.80%	7.966%
10	5.918	1508	1517	1532	rVB7	2676	5536	1.23%	0.152%
11	6.069	1551	1564	1589	rBV	101828	213639	47.58%	5.849%
12	6.989	1840	1850	1873	rBV	44131	86002	19.15%	2.355%
13	7.317	1941	1952	1972	rBV	208044	366766	81.68%	10.042%
14	7.628	2039	2049	2066	rBV	26484	50133	11.17%	1.373%
15	8.091	2178	2193	2228	rBV	168276	351317	78.24%	9.619%
16	8.854	2419	2430	2455	rBV	226903	371949	82.84%	10.184%
17	10.217	2843	2854	2873	rBV	70886	114629	25.53%	3.139%
18	11.249	3164	3175	3190	rBV	212896	328535	73.17%	8.995%
19	11.625	3281	3292	3307	rBV	202167	315583	70.29%	8.641%




Sum of corrected areas: 3652334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023237.D
Acq On : 05 Nov 2021 17:10
Operator : SY/MD
Sample : M4535-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

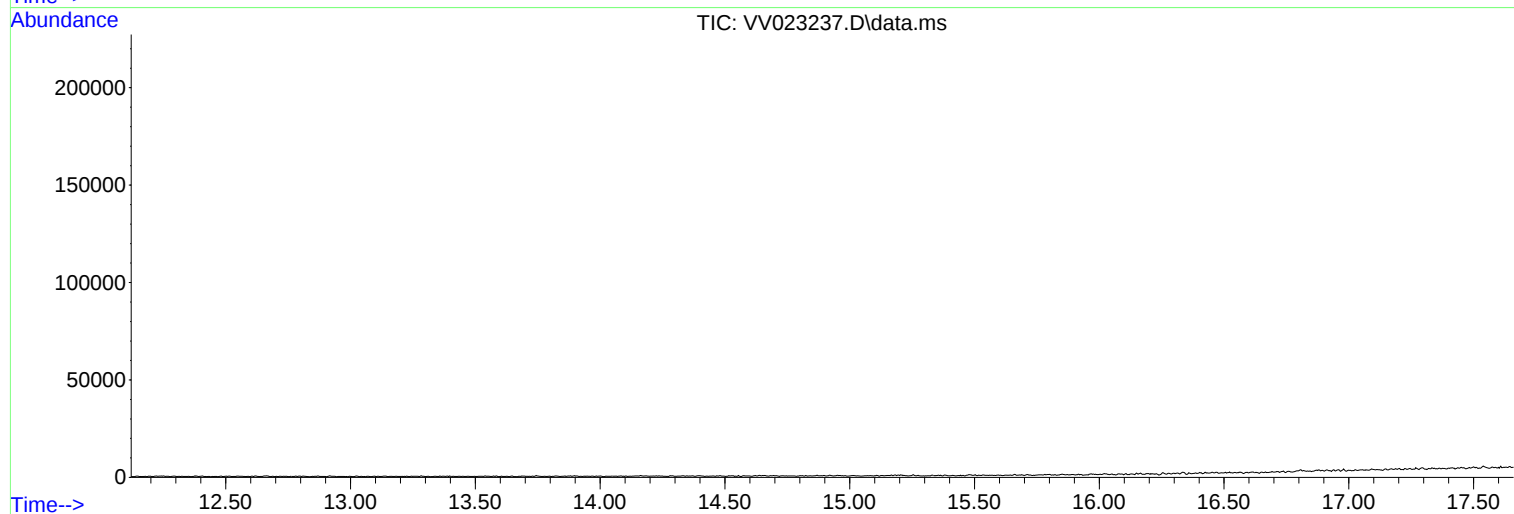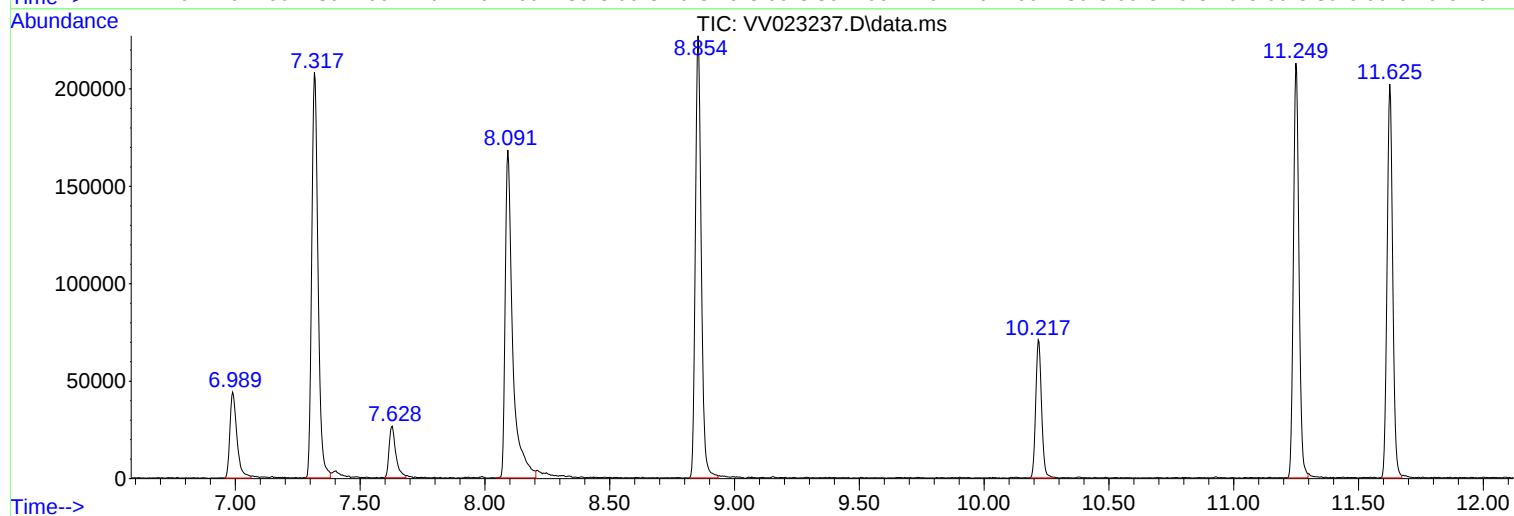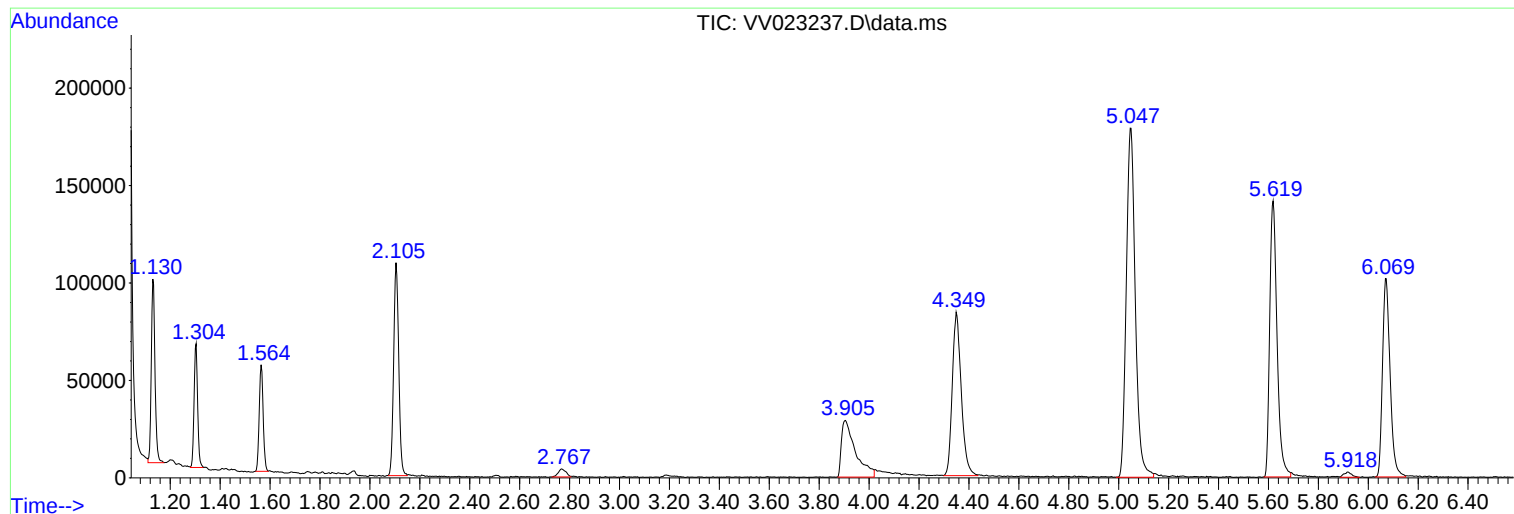

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023237.D
Acq On : 05 Nov 2021 17:10
Operator : SY/MD
Sample : M4535-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023237.D
Acq On : 05 Nov 2021 17:10
Operator : SY/MD
Sample : M4535-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4621

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc