

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023240.D
 Acq On : 05 Nov 2021 18:20
 Operator : SY/MD
 Sample : M4535-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	42	rVB	99084	99537	20.99%	2.368%
2	1.307	76	83	93	rBV	68716	67981	14.33%	1.617%
3	1.568	156	164	177	rBV	60263	67397	14.21%	1.603%
4	2.108	322	332	350	rBV	116425	169111	35.66%	4.023%
5	2.773	525	539	547	rBV5	6476	13292	2.80%	0.316%
6	3.895	878	888	930	rBV	48628	182608	38.50%	4.344%
7	4.349	1014	1029	1054	rBV	85647	223629	47.15%	5.320%
8	5.050	1229	1247	1274	rBV3	187782	474294	100.00%	11.283%
9	5.619	1413	1424	1446	rBV	150949	304861	64.28%	7.252%
10	5.921	1506	1518	1538	rBV4	23738	52366	11.04%	1.246%
11	6.072	1551	1565	1594	rBV	107473	227775	48.02%	5.419%
12	6.989	1840	1850	1869	rBV	47925	90127	19.00%	2.144%
13	7.317	1939	1952	1971	rBV	220364	392146	82.68%	9.329%
14	7.628	2038	2049	2069	rBV	29170	54312	11.45%	1.292%
15	7.976	2146	2157	2181	rVB	119417	200801	42.34%	4.777%
16	8.091	2183	2193	2220	rBV	202986	386850	81.56%	9.203%
17	8.853	2417	2430	2447	rBV	234277	383146	80.78%	9.115%
18	10.217	2840	2854	2870	rBV	74081	120029	25.31%	2.855%
19	11.249	3165	3175	3195	rBV	226434	352912	74.41%	8.395%
20	11.625	3281	3292	3310	rBV	214897	340430	71.78%	8.099%




Sum of corrected areas: 4203604

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023240.D
Acq On : 05 Nov 2021 18:20
Operator : SY/MD
Sample : M4535-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

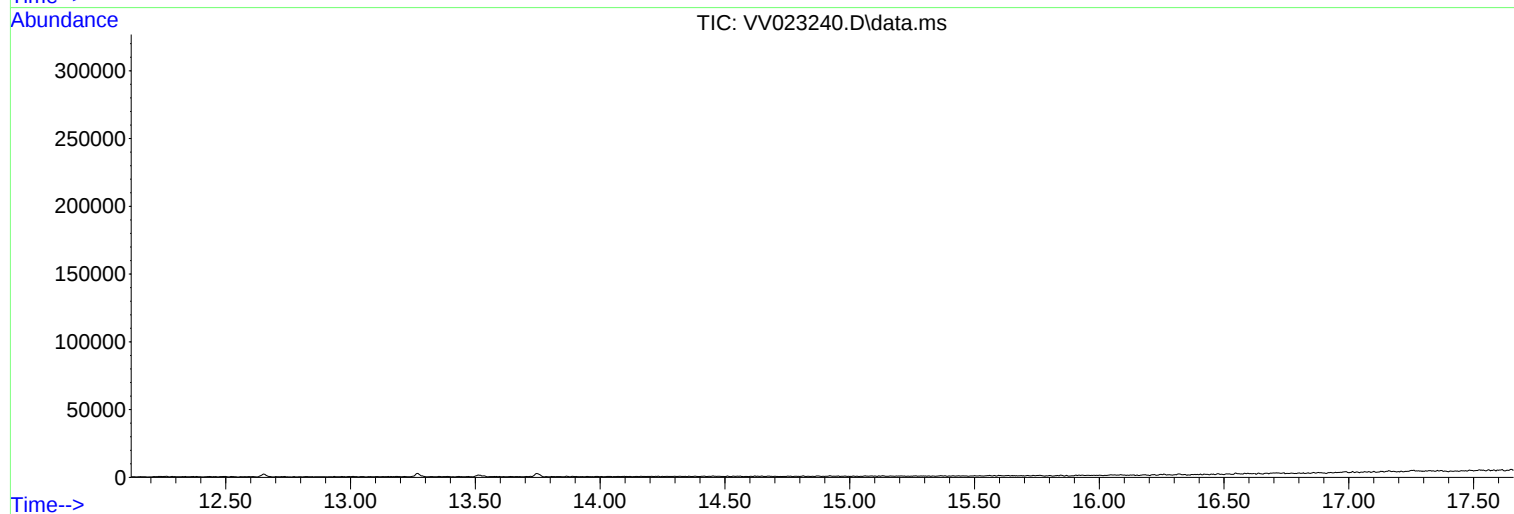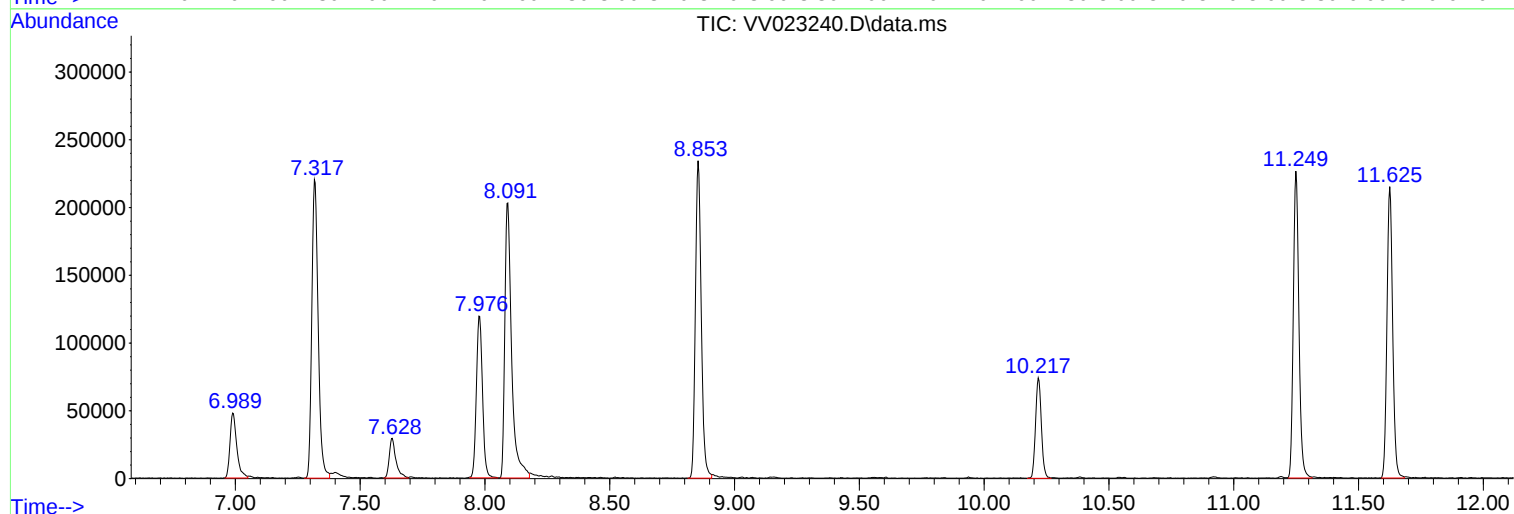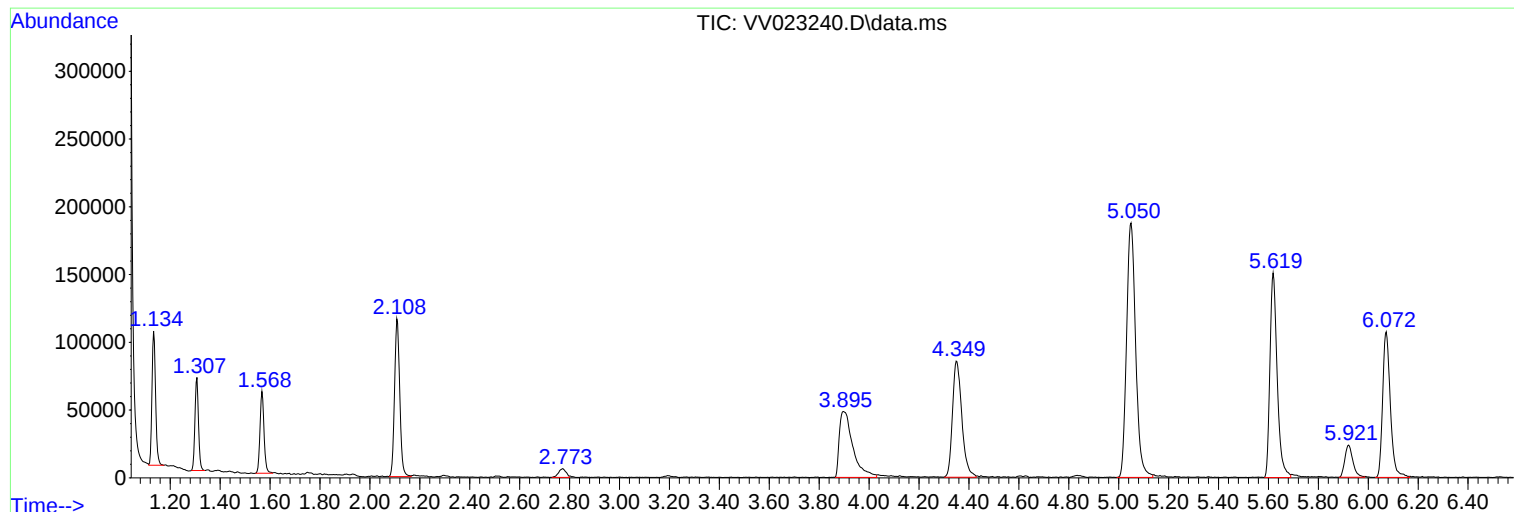

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023240.D
Acq On : 05 Nov 2021 18:20
Operator : SY/MD
Sample : M4535-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023240.D
Acq On : 05 Nov 2021 18:20
Operator : SY/MD
Sample : M4535-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc