

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023242.D
 Acq On : 05 Nov 2021 19:07
 Operator : SY/MD
 Sample : M4535-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	23	29	45	rVB	180098	180650	20.81%	3.452%
2	1.307	76	83	92	rBV	71077	69083	7.96%	1.320%
3	1.568	157	164	173	rBV	60840	66386	7.65%	1.269%
4	2.111	322	333	346	rBV	119023	169977	19.58%	3.248%
5	2.770	521	538	564	rBV	98739	209215	24.11%	3.998%
6	3.886	876	885	917	rBV2	53616	181802	20.95%	3.474%
7	4.355	1013	1031	1054	rBV	87707	220718	25.43%	4.218%
8	5.050	1229	1247	1272	rBV2	195265	488340	56.27%	9.332%
9	5.619	1412	1424	1449	rBV	149464	301870	34.78%	5.769%
10	5.918	1506	1517	1533	rBV2	54802	113004	13.02%	2.159%
11	6.072	1552	1565	1594	rBV	112502	233858	26.94%	4.469%
12	6.989	1839	1850	1867	rBV	50321	91875	10.59%	1.756%
13	7.316	1941	1952	1971	rBV	226167	400750	46.17%	7.658%
14	7.628	2039	2049	2064	rBV	28421	51902	5.98%	0.992%
15	7.976	2141	2157	2174	rBV	518245	867916	100.00%	16.586%
16	8.088	2183	2192	2227	rBV	213288	393069	45.29%	7.511%
17	8.853	2417	2430	2448	rBV	230414	379125	43.68%	7.245%
18	10.217	2842	2854	2871	rBV2	74284	119724	13.79%	2.288%
19	11.249	3164	3175	3193	rBV	222641	347104	39.99%	6.633%
20	11.625	3279	3292	3313	rBV	217165	346553	39.93%	6.623%




Sum of corrected areas: 5232921

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023242.D
Acq On : 05 Nov 2021 19:07
Operator : SY/MD
Sample : M4535-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

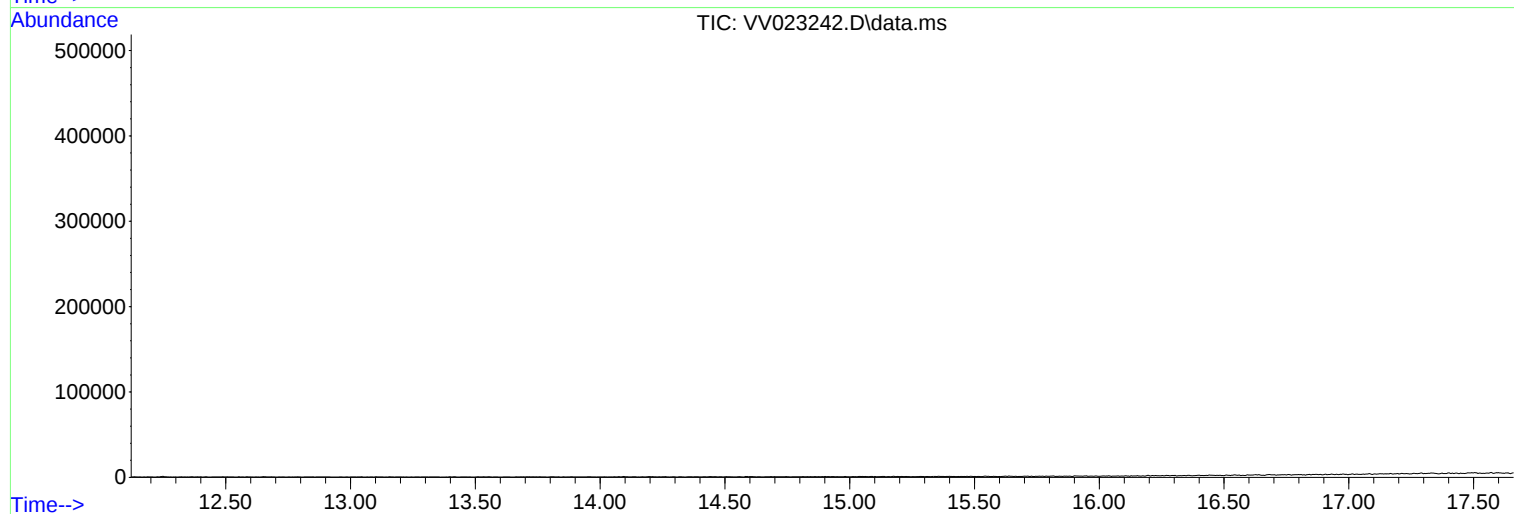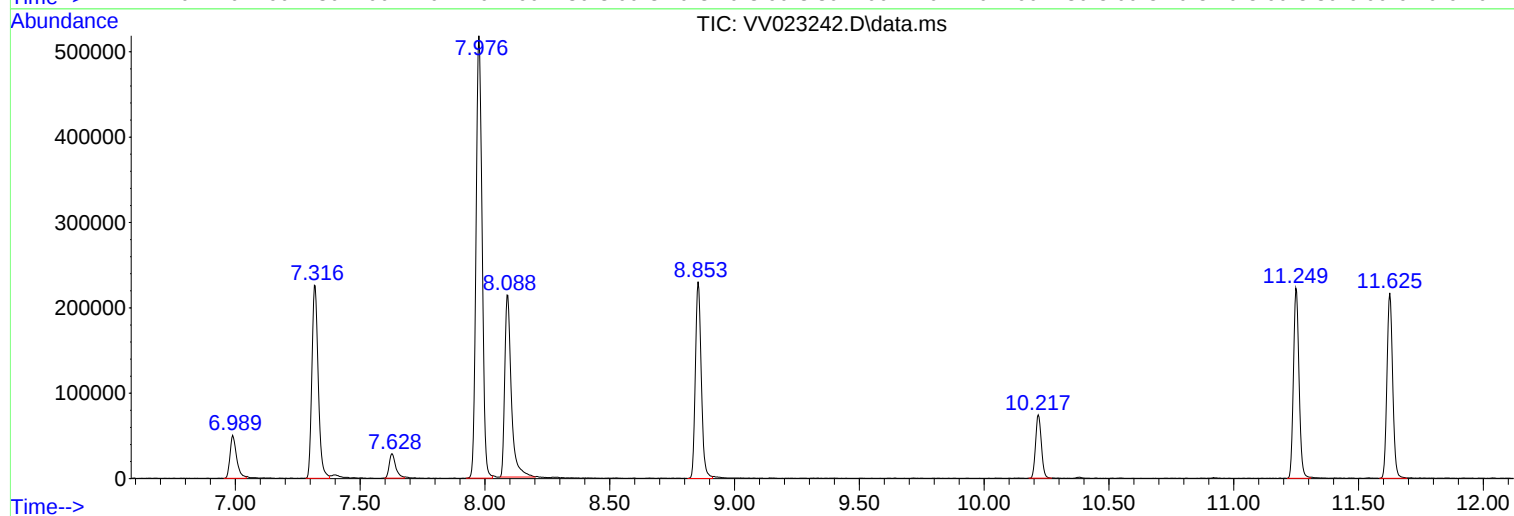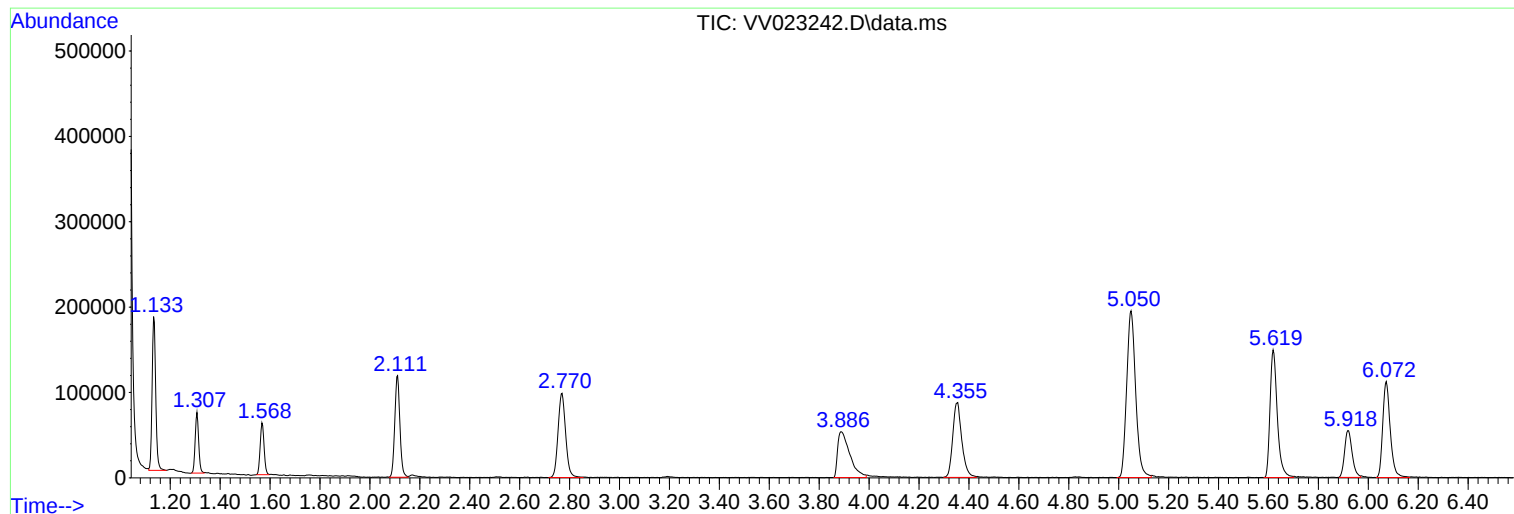

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023242.D
Acq On : 05 Nov 2021 19:07
Operator : SY/MD
Sample : M4535-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023242.D
Acq On : 05 Nov 2021 19:07
Operator : SY/MD
Sample : M4535-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc