

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023243.D
 Acq On : 05 Nov 2021 19:31
 Operator : SY/MD
 Sample : M4535-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4625

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	44	rVB	256909	254740	49.36%	5.560%
2	1.307	76	83	93	rVB	69877	68841	13.34%	1.502%
3	1.568	157	164	177	rVB	61386	67116	13.01%	1.465%
4	2.108	322	332	347	rBV	117093	167607	32.48%	3.658%
5	3.889	876	886	912	rBV	48921	150113	29.09%	3.276%
6	4.352	1012	1030	1056	rBV	85000	214665	41.60%	4.685%
7	5.050	1231	1247	1279	rBV3	185657	475698	92.18%	10.382%
8	5.619	1412	1424	1448	rBV	144126	297028	57.56%	6.483%
9	5.921	1507	1518	1541	rVB6	16775	37811	7.33%	0.825%
10	6.072	1552	1565	1594	rBV	110054	231656	44.89%	5.056%
11	6.989	1838	1850	1865	rBV	47910	89448	17.33%	1.952%
12	7.317	1941	1952	1972	rBV	224411	391649	75.89%	8.548%
13	7.625	2036	2048	2068	rBV	29392	53631	10.39%	1.171%
14	7.976	2137	2157	2177	rBV	301251	516048	100.00%	11.263%
15	8.088	2183	2192	2227	rBV	205748	385556	74.71%	8.415%
16	8.854	2419	2430	2451	rBV	228609	378840	73.41%	8.268%
17	10.217	2842	2854	2874	rBV	75304	118970	23.05%	2.597%
18	11.249	3164	3175	3192	rBV	218787	344573	66.77%	7.520%
19	11.625	3281	3292	3309	rBV	214744	337823	65.46%	7.373%




Sum of corrected areas: 4581813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023243.D
Acq On : 05 Nov 2021 19:31
Operator : SY/MD
Sample : M4535-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

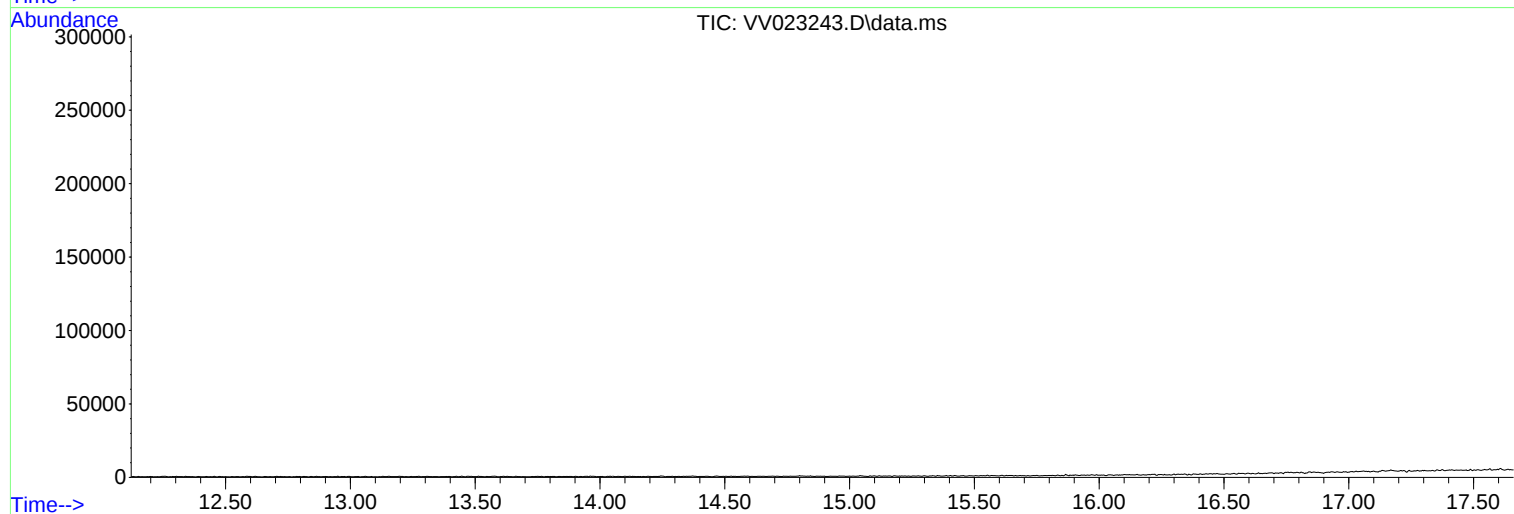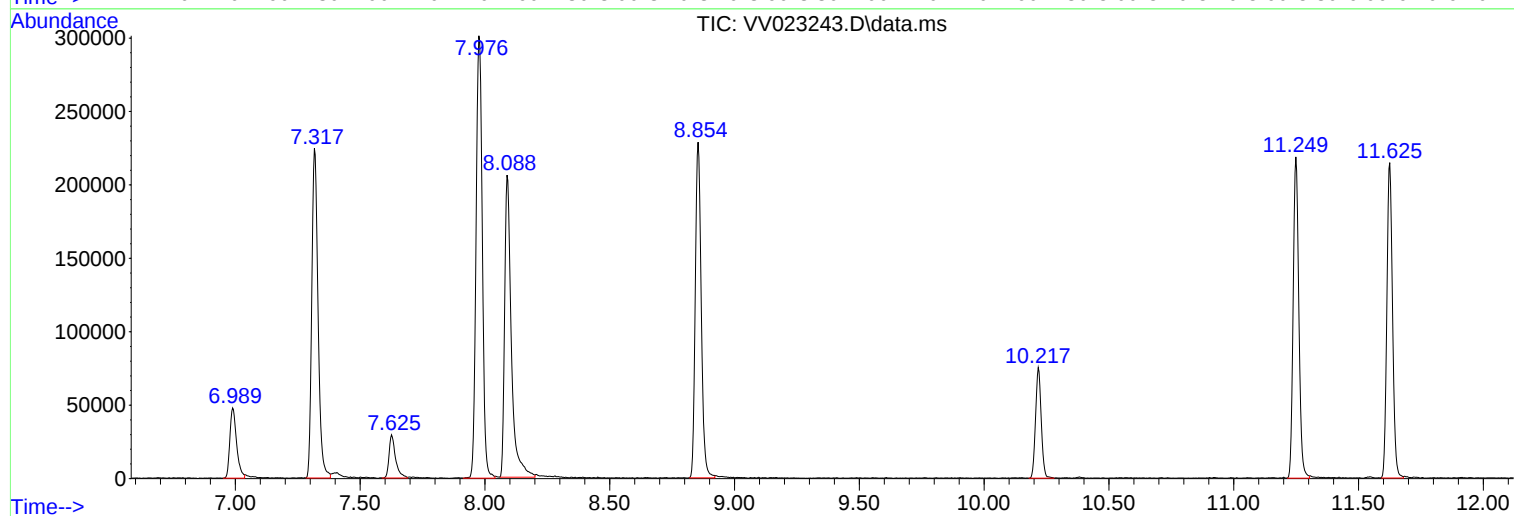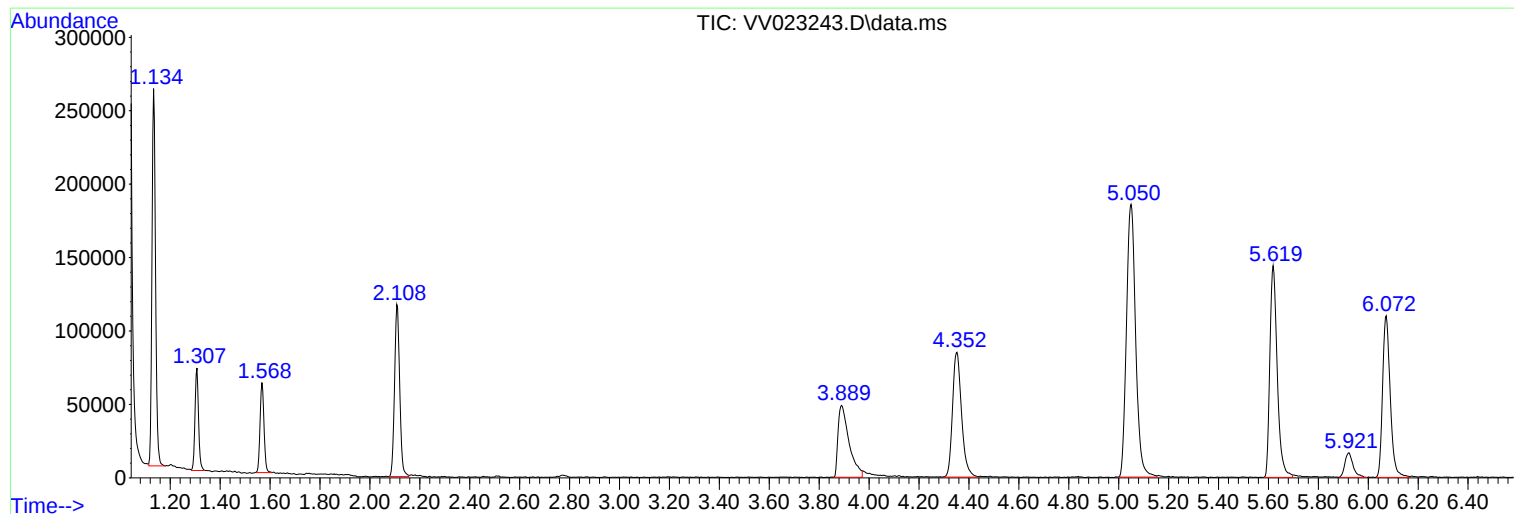

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023243.D
Acq On : 05 Nov 2021 19:31
Operator : SY/MD
Sample : M4535-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023243.D
Acq On : 05 Nov 2021 19:31
Operator : SY/MD
Sample : M4535-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc