

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023244.D
 Acq On : 05 Nov 2021 19:54
 Operator : SY/MD
 Sample : M4535-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4626

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	41	rVB	28689	30293	3.60%	0.644%
2	1.307	76	83	99	rVB	69018	71449	8.48%	1.518%
3	1.568	157	164	177	rBV	58585	65431	7.77%	1.390%
4	2.111	320	333	348	rBV	112467	169615	20.13%	3.604%
5	3.902	879	890	921	rBV	41148	148505	17.63%	3.155%
6	4.349	1012	1029	1057	rBV2	85929	218922	25.99%	4.652%
7	5.050	1230	1247	1272	rBV3	186093	464228	55.11%	9.864%
8	5.619	1412	1424	1444	rBV	146666	301192	35.75%	6.400%
9	5.921	1506	1518	1542	rBV3	40146	87171	10.35%	1.852%
10	6.072	1553	1565	1591	rBV	108725	223619	26.55%	4.751%
11	6.989	1840	1850	1867	rBV	47034	86357	10.25%	1.835%
12	7.317	1941	1952	1970	rBV	215730	382626	45.42%	8.130%
13	7.625	2039	2048	2070	rBV	27794	52208	6.20%	1.109%
14	7.976	2145	2157	2181	rBV	505466	842407	100.00%	17.899%
15	8.091	2184	2193	2224	rBV	201395	382251	45.38%	8.122%
16	8.853	2416	2430	2452	rBV	233996	385203	45.73%	8.185%
17	10.217	2841	2854	2870	rBV	72336	116669	13.85%	2.479%
18	11.249	3164	3175	3192	rBV	222529	349240	41.46%	7.421%
19	11.625	3281	3292	3309	rBV	207811	329010	39.06%	6.991%




Sum of corrected areas: 4706396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023244.D
Acq On : 05 Nov 2021 19:54
Operator : SY/MD
Sample : M4535-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

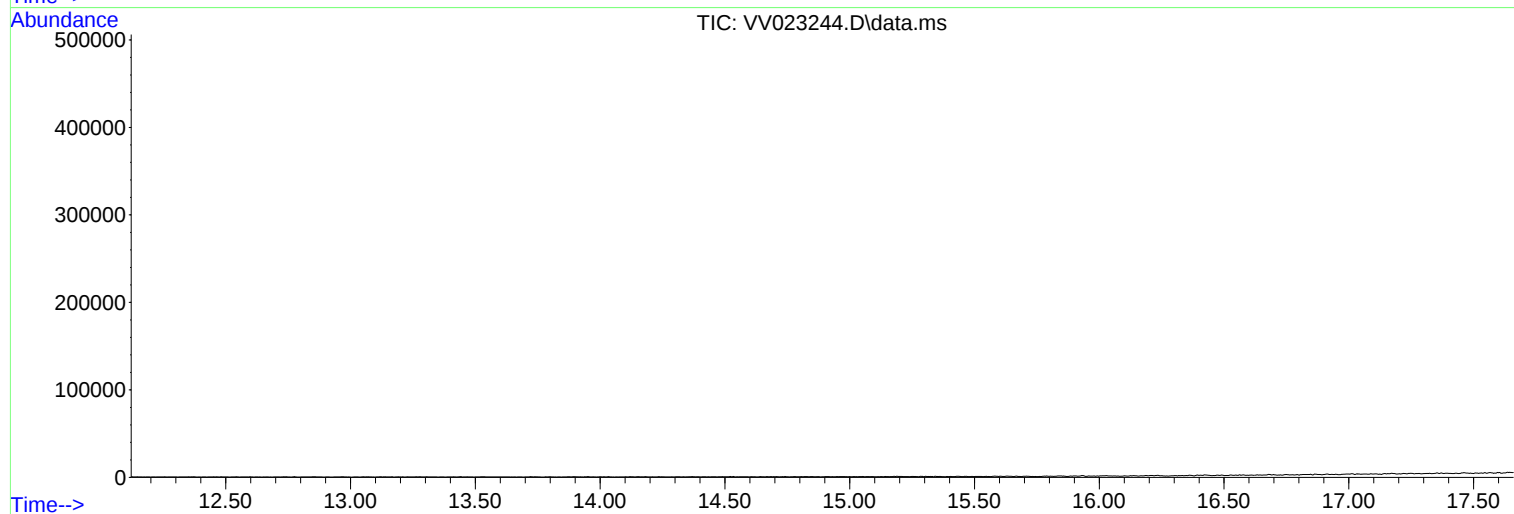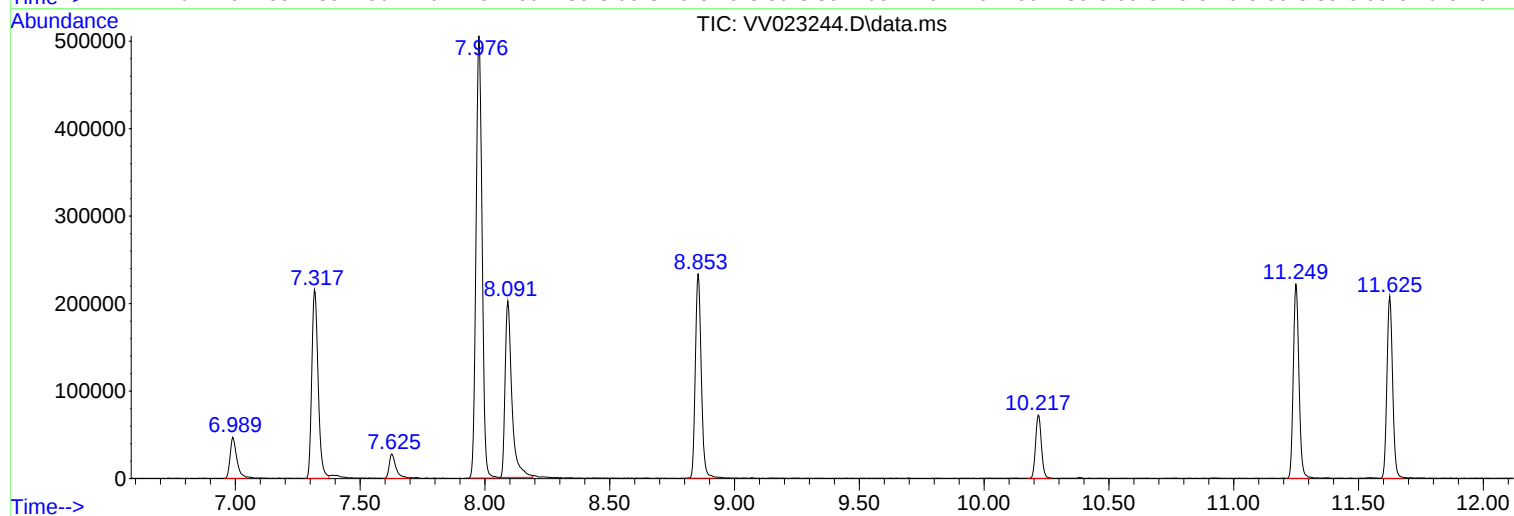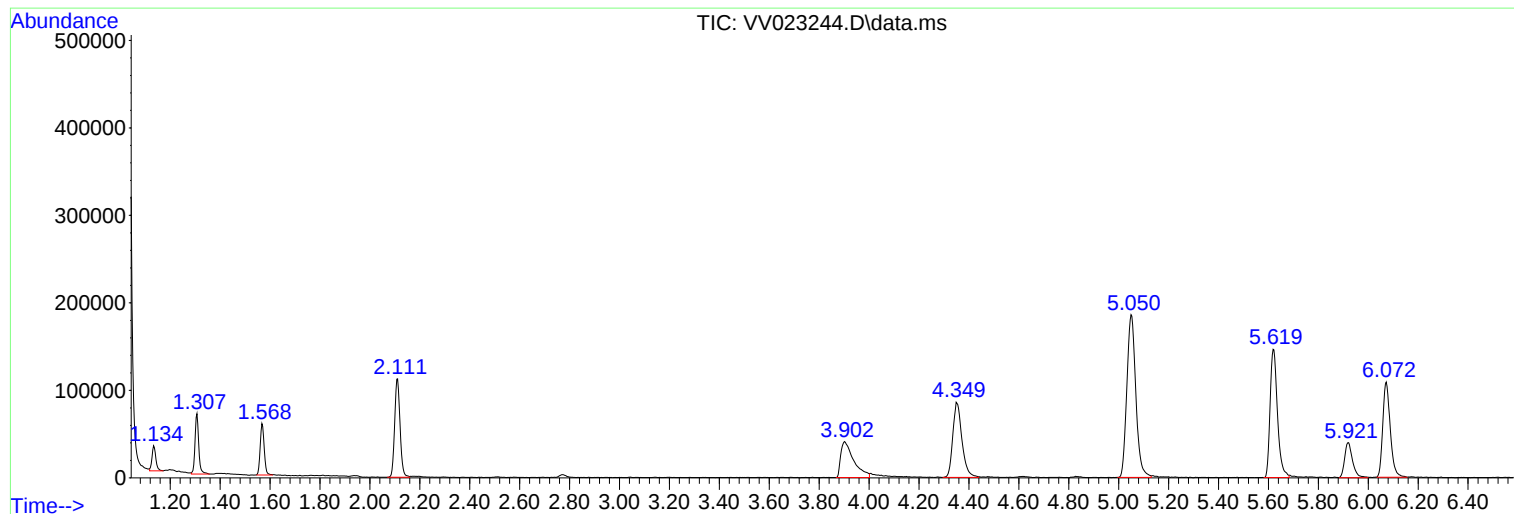

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023244.D
Acq On : 05 Nov 2021 19:54
Operator : SY/MD
Sample : M4535-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4626










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Difluorochloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.134	0.50 ug/L	30293	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Difluorochloromethane	86	CHClF2	000075-45-6	91
2			Difluorochloromethane	86	CHClF2	000075-45-6	90
3			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	7
4			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	5
5			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	5

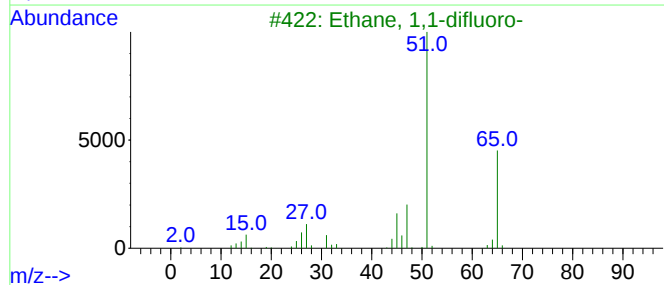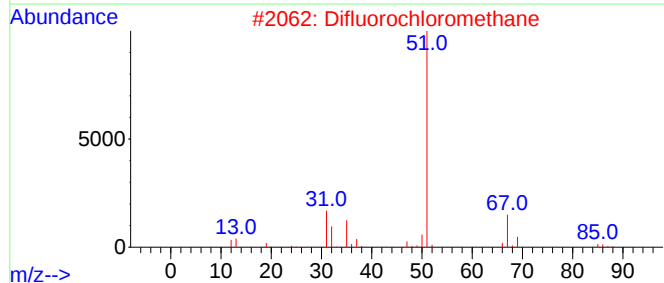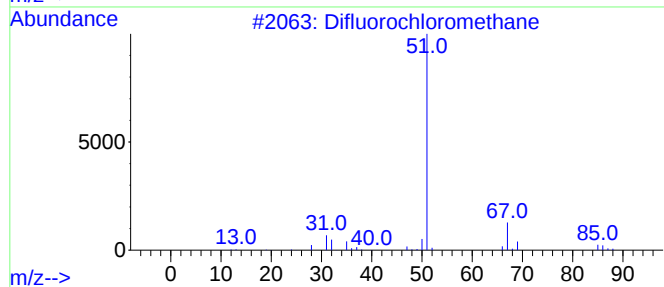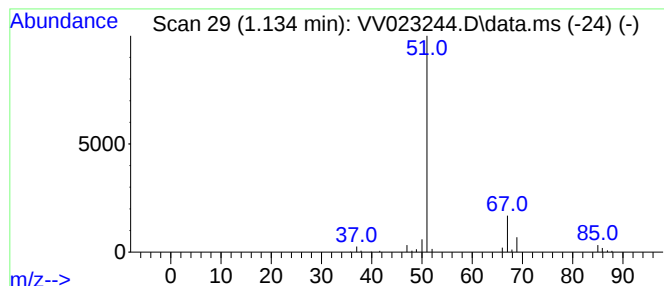

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023244.D
Acq On : 05 Nov 2021 19:54
Operator : SY/MD
Sample : M4535-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Difluorochlorom...	1.134	0.5	ug/L	30293	1	5.619	301192	5.0