

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023245.D
 Acq On : 05 Nov 2021 20:18
 Operator : SY/MD
 Sample : M4535-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4627

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	36	rVB	27889	26508	3.51%	0.603%
2	1.307	76	83	91	rBV	64317	63730	8.45%	1.449%
3	1.568	156	164	176	rBV	57253	63527	8.42%	1.444%
4	2.108	322	332	348	rBV	107225	158043	20.95%	3.593%
5	3.899	879	889	921	rBV	37077	130883	17.35%	2.976%
6	4.349	1013	1029	1055	rBV2	81342	211063	27.98%	4.799%
7	5.050	1228	1247	1275	rBV3	182218	456712	60.55%	10.383%
8	5.619	1412	1424	1447	rBV	132995	273929	36.32%	6.228%
9	5.918	1500	1517	1536	rBV3	35935	79130	10.49%	1.799%
10	6.072	1552	1565	1590	rBV	105364	220161	29.19%	5.005%
11	6.989	1841	1850	1875	rBV	45340	87100	11.55%	1.980%
12	7.317	1938	1952	1973	rBV	204424	359328	47.64%	8.169%
13	7.625	2037	2048	2071	rBV2	26728	51511	6.83%	1.171%
14	7.976	2144	2157	2177	rBV	453278	754312	100.00%	17.149%
15	8.091	2183	2193	2232	rBV	186561	383069	50.78%	8.709%
16	8.854	2419	2430	2448	rBV	209235	343335	45.52%	7.806%
17	10.217	2843	2854	2869	rBV	75060	119221	15.81%	2.711%
18	11.249	3160	3175	3194	rBV	195134	307446	40.76%	6.990%
19	11.625	3281	3292	3308	rBV	197641	309461	41.03%	7.036%




Sum of corrected areas: 4398469

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023245.D
Acq On : 05 Nov 2021 20:18
Operator : SY/MD
Sample : M4535-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

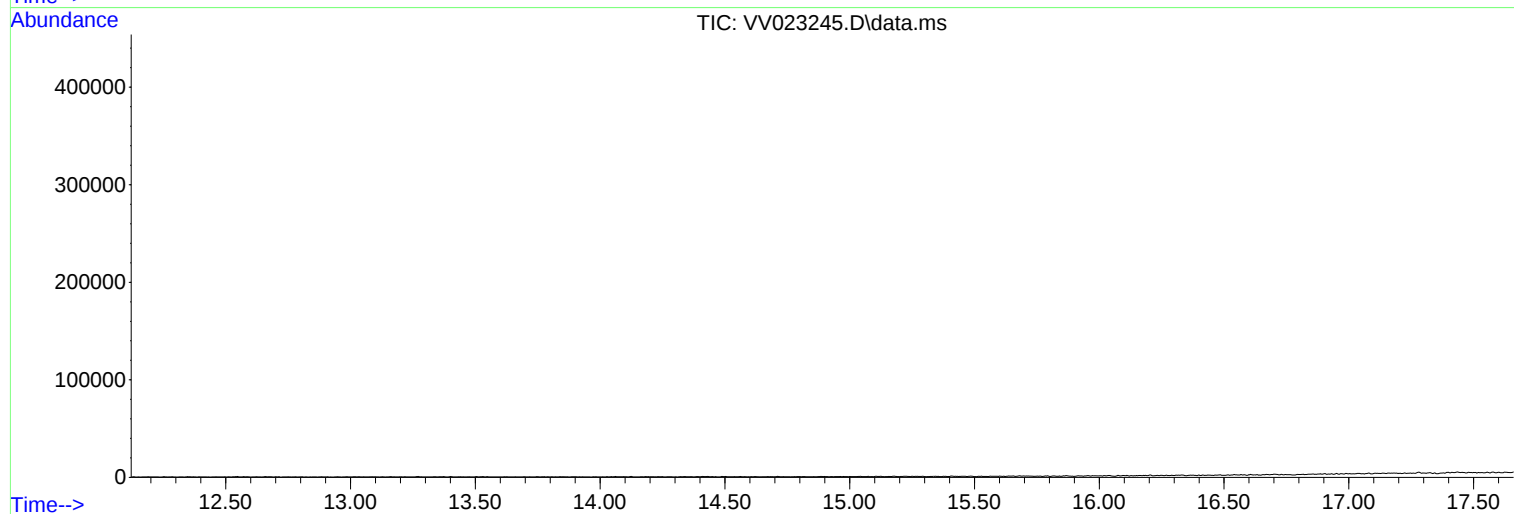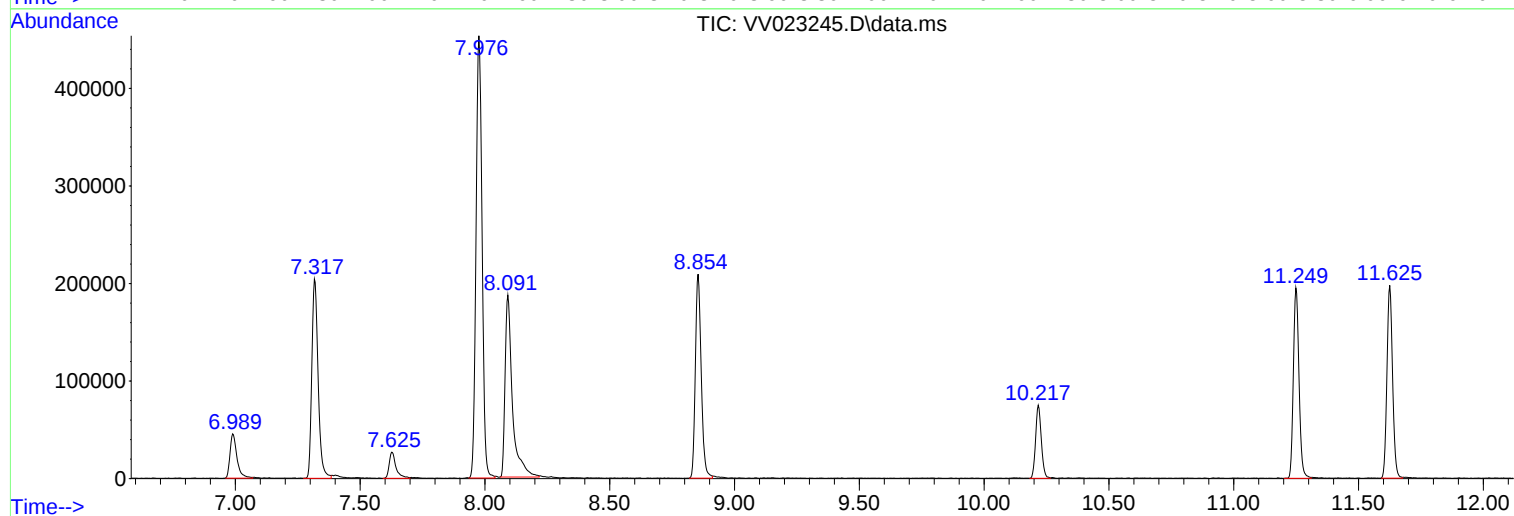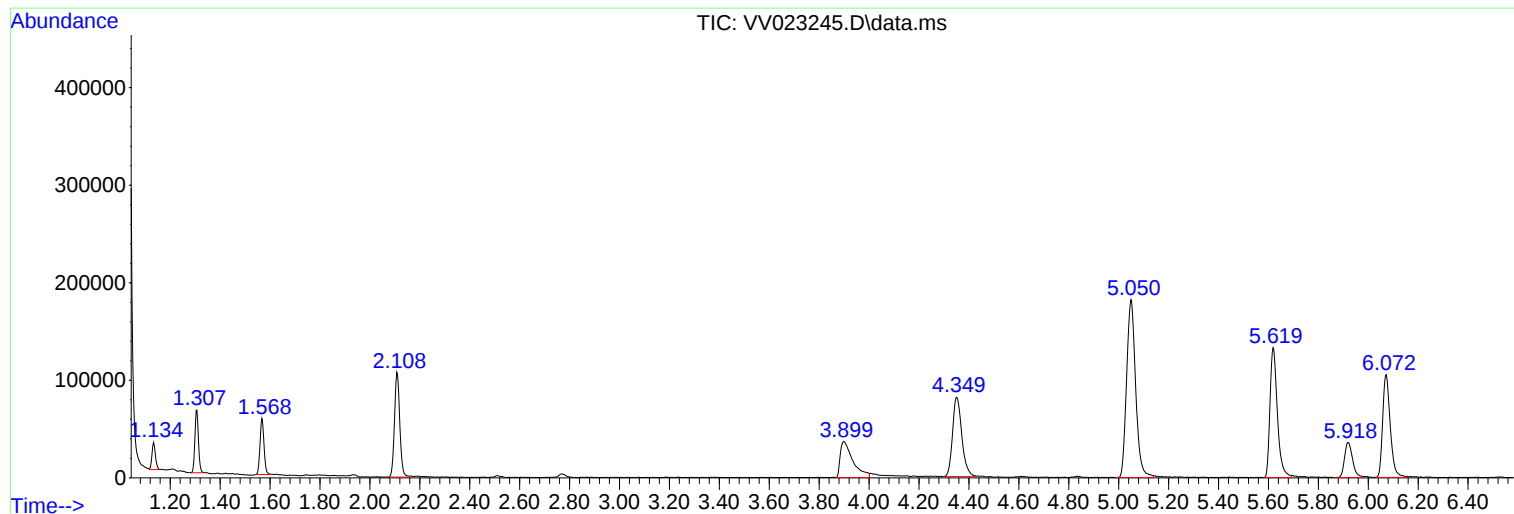

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023245.D
Acq On : 05 Nov 2021 20:18
Operator : SY/MD
Sample : M4535-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023245.D
Acq On : 05 Nov 2021 20:18
Operator : SY/MD
Sample : M4535-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
