

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023248.D
 Acq On : 05 Nov 2021 21:51
 Operator : SY/MD
 Sample : M4535-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4565

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	21	25	37	rVB	5985	6884	1.65%	0.187%
2	1.307	76	83	101	rVB	60806	62247	14.89%	1.687%
3	1.568	156	164	175	rBV	52719	60116	14.38%	1.629%
4	2.111	322	333	347	rBV	98467	142579	34.11%	3.865%
5	2.182	347	355	367	rVB4	3009	7079	1.69%	0.192%
6	2.297	381	391	405	rVB	103644	151825	36.32%	4.115%
7	3.899	873	889	923	rBV2	41791	148452	35.51%	4.024%
8	4.352	1014	1030	1054	rBV	74343	189273	45.28%	5.130%
9	5.050	1231	1247	1276	rBV2	166531	418015	100.00%	11.330%
10	5.619	1412	1424	1453	rBV	145988	301384	72.10%	8.169%
11	5.915	1505	1516	1529	rBV6	5210	11670	2.79%	0.316%
12	6.072	1552	1565	1587	rBV	97148	201671	48.24%	5.466%
13	6.989	1839	1850	1875	rBV	42926	83458	19.97%	2.262%
14	7.316	1940	1952	1971	rBV	188455	337188	80.66%	9.139%
15	7.628	2038	2049	2068	rBV3	26930	50778	12.15%	1.376%
16	8.091	2183	2193	2229	rBV2	174964	355214	84.98%	9.628%
17	8.853	2417	2430	2461	rBV	233334	381987	91.38%	10.354%
18	10.217	2843	2854	2871	rBV	62512	99870	23.89%	2.707%
19	11.249	3165	3175	3192	rBV	224178	343574	82.19%	9.312%
20	11.625	3279	3292	3316	rBV	188145	296665	70.97%	8.041%
21	12.252	3478	3487	3496	rVB2	6050	8376	2.00%	0.227%
22	12.345	3508	3516	3529	rBV5	7363	10927	2.61%	0.296%
23	14.043	4034	4044	4056	rVB2	11813	20180	4.83%	0.547%




Sum of corrected areas: 3689412

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023248.D
Acq On : 05 Nov 2021 21:51
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

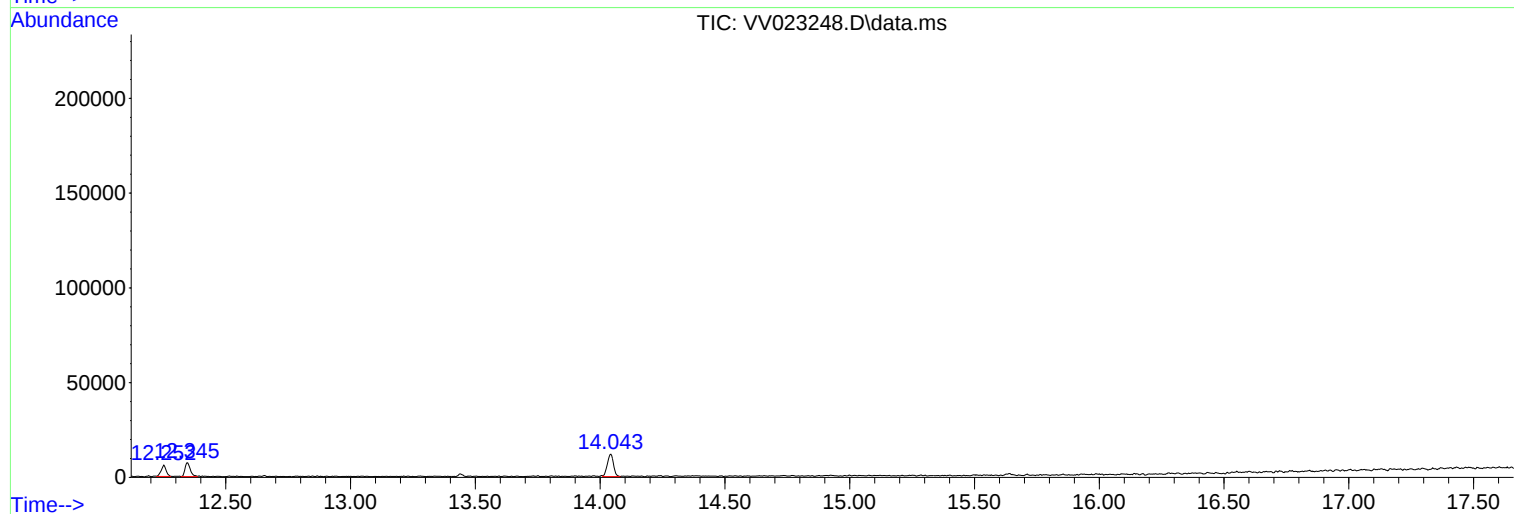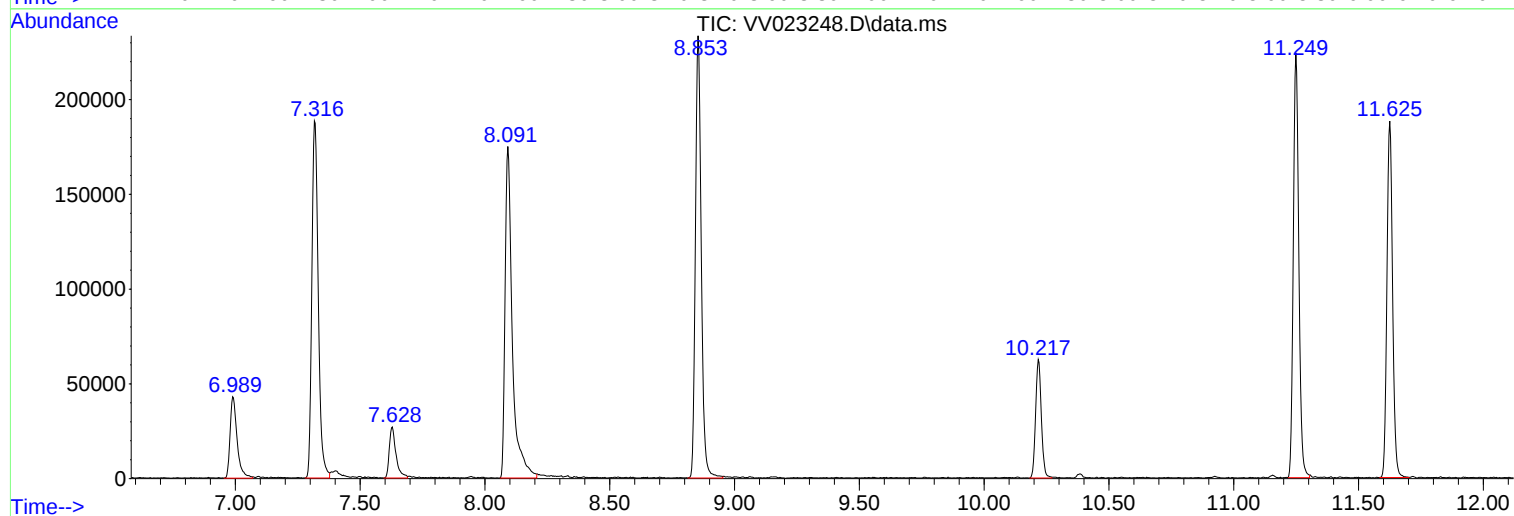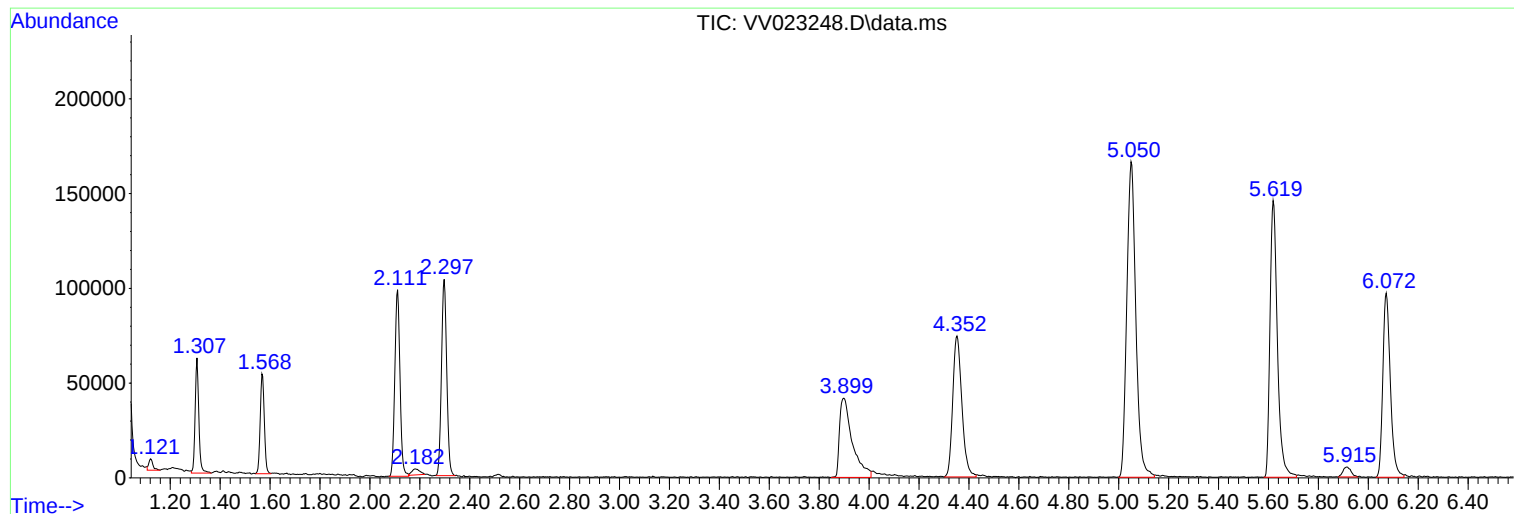

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023248.D
Acq On : 05 Nov 2021 21:51
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023248.D
Acq On : 05 Nov 2021 21:51
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc