

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023249.D
 Acq On : 05 Nov 2021 22:15
 Operator : SY/MD
 Sample : M4535-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4570

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	59058	60514	14.39%	1.735%
2	1.568	156	164	182	rBV	53872	61667	14.67%	1.768%
3	2.111	322	333	347	rBV	98548	145113	34.51%	4.160%
4	2.179	347	354	368	rVB2	3526	7980	1.90%	0.229%
5	3.889	875	886	908	rBV2	43481	128620	30.59%	3.687%
6	4.352	1015	1030	1059	rBV2	75812	191248	45.49%	5.483%
7	5.050	1229	1247	1275	rBV3	165651	420462	100.00%	12.054%
8	5.619	1412	1424	1446	rBV	145840	299633	71.26%	8.590%
9	5.912	1506	1515	1516	rBV4	5263	5637	1.34%	0.162%
10	6.072	1551	1565	1592	rBV2	95152	203419	48.38%	5.832%
11	6.989	1839	1850	1872	rBV	44889	84803	20.17%	2.431%
12	7.317	1941	1952	1972	rBV	190395	339273	80.69%	9.727%
13	7.625	2039	2048	2068	rBV2	26411	47658	11.33%	1.366%
14	8.092	2183	2193	2222	rBV2	171378	336948	80.14%	9.660%
15	8.854	2416	2430	2451	rBV	226043	377465	89.77%	10.822%
16	10.217	2841	2854	2870	rBV	60560	96201	22.88%	2.758%
17	10.381	2897	2905	2917	rVB4	3263	5386	1.28%	0.154%
18	11.249	3164	3175	3195	rBV	224357	342306	81.41%	9.814%
19	11.625	3280	3292	3309	rBV	189705	299080	71.13%	8.574%
20	12.252	3476	3487	3496	rBV	7960	12032	2.86%	0.345%
21	14.040	4030	4043	4057	rBV	13816	22625	5.38%	0.649%




Sum of corrected areas: 3488070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023249.D
Acq On : 05 Nov 2021 22:15
Operator : SY/MD
Sample : M4535-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4570

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

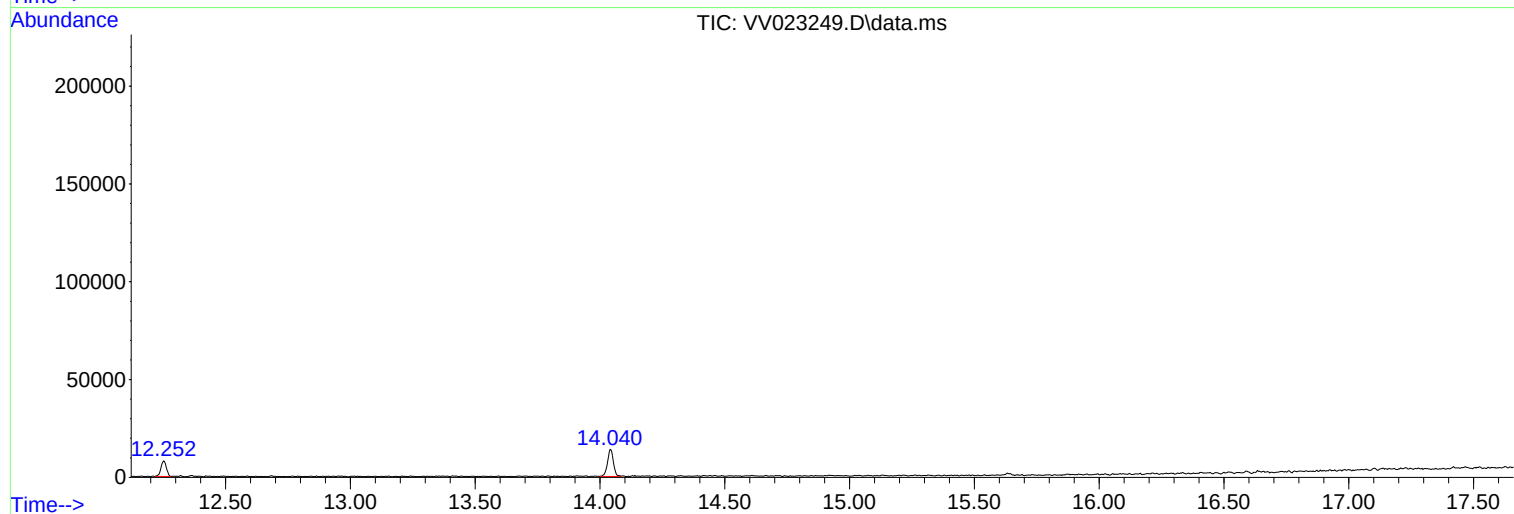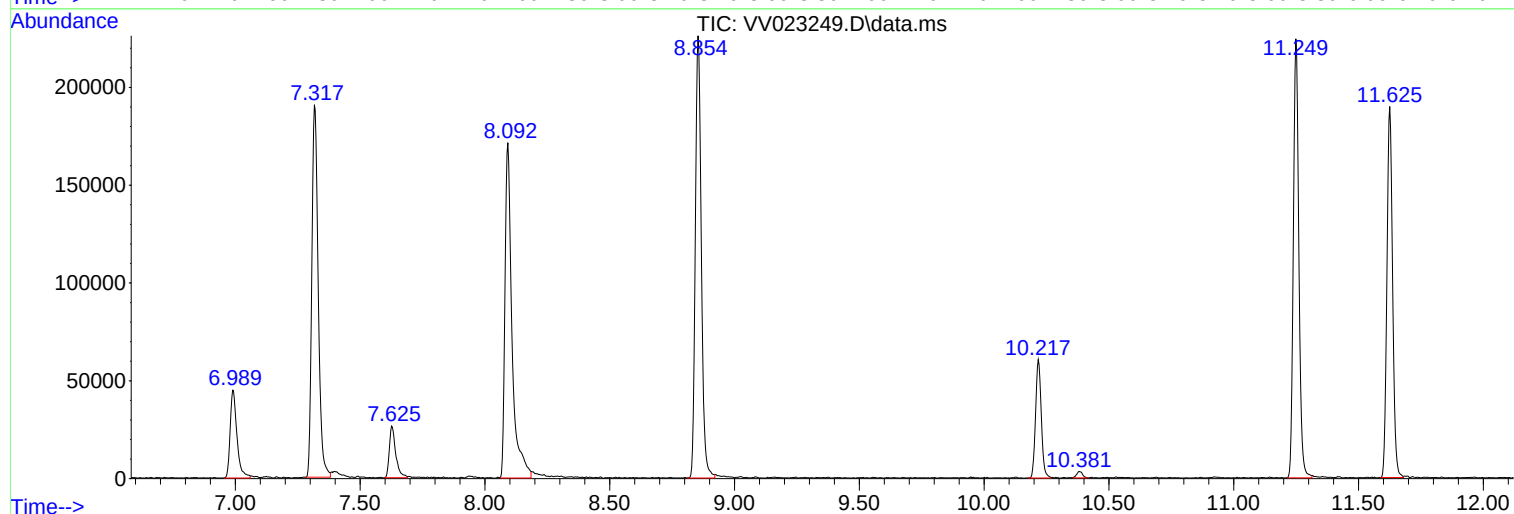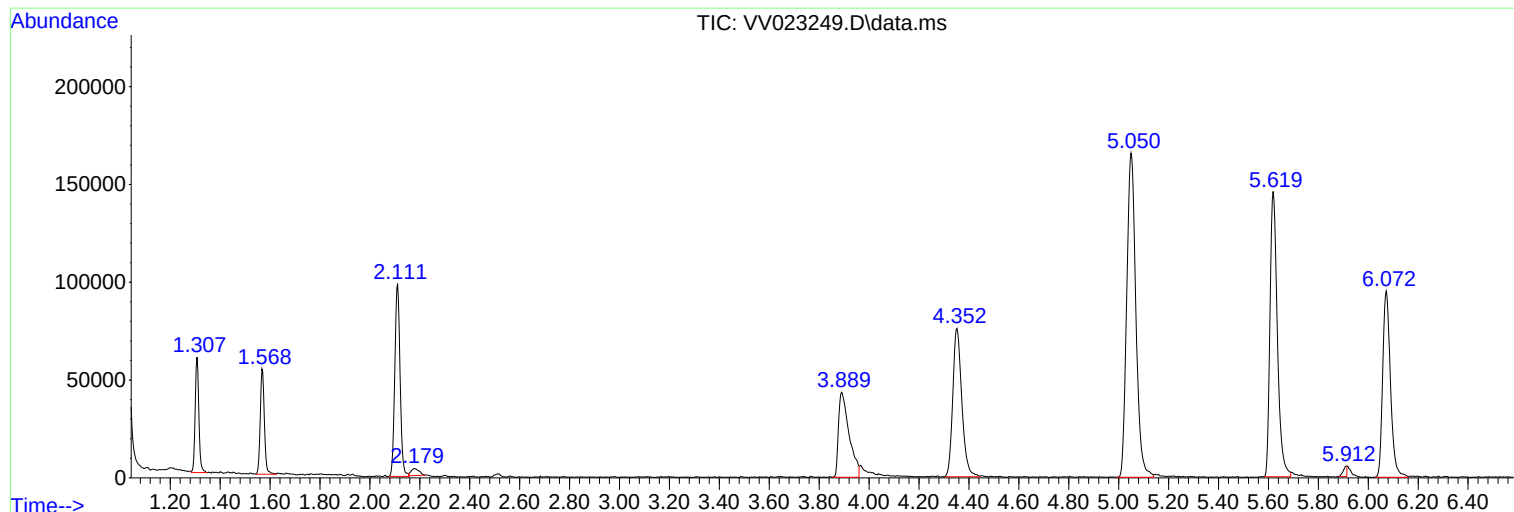

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023249.D
Acq On : 05 Nov 2021 22:15
Operator : SY/MD
Sample : M4535-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4570

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023249.D
Acq On : 05 Nov 2021 22:15
Operator : SY/MD
Sample : M4535-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4570

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
