

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023254.D
 Acq On : 06 Nov 2021 00:11
 Operator : SY/MD
 Sample : M4535-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4602

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	22	29	43	rVB	414362	406759	96.02%	9.467%
2	1.307	76	83	96	rVB	58845	60425	14.26%	1.406%
3	1.568	154	164	174	rBV	54229	61840	14.60%	1.439%
4	2.111	323	333	349	rBV	99323	146131	34.49%	3.401%
5	3.889	877	886	919	rBV2	45025	141988	33.52%	3.305%
6	4.352	1014	1030	1058	rBV	78416	196135	46.30%	4.565%
7	5.050	1231	1247	1272	rBV3	168124	423637	100.00%	9.860%
8	5.619	1411	1424	1451	rBV	146355	303046	71.53%	7.053%
9	5.924	1507	1519	1538	rVB7	11490	26333	6.22%	0.613%
10	6.072	1548	1565	1587	rBV	100891	207440	48.97%	4.828%
11	6.989	1839	1850	1867	rBV2	43117	81666	19.28%	1.901%
12	7.317	1941	1952	1972	rBV	195082	342073	80.75%	7.962%
13	7.628	2039	2049	2072	rBV3	26797	50674	11.96%	1.179%
14	7.976	2142	2157	2174	rBV	204952	346010	81.68%	8.053%
15	8.091	2182	2193	2224	rBV	186619	359292	84.81%	8.363%
16	8.853	2419	2430	2452	rBV	229885	380123	89.73%	8.847%
17	10.217	2843	2854	2878	rVB	69025	110976	26.20%	2.583%
18	11.249	3165	3175	3196	rBV	222393	345893	81.65%	8.051%
19	11.625	3280	3292	3310	rBV	194339	305963	72.22%	7.121%




Sum of corrected areas: 4296404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023254.D
Acq On : 06 Nov 2021 00:11
Operator : SY/MD
Sample : M4535-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

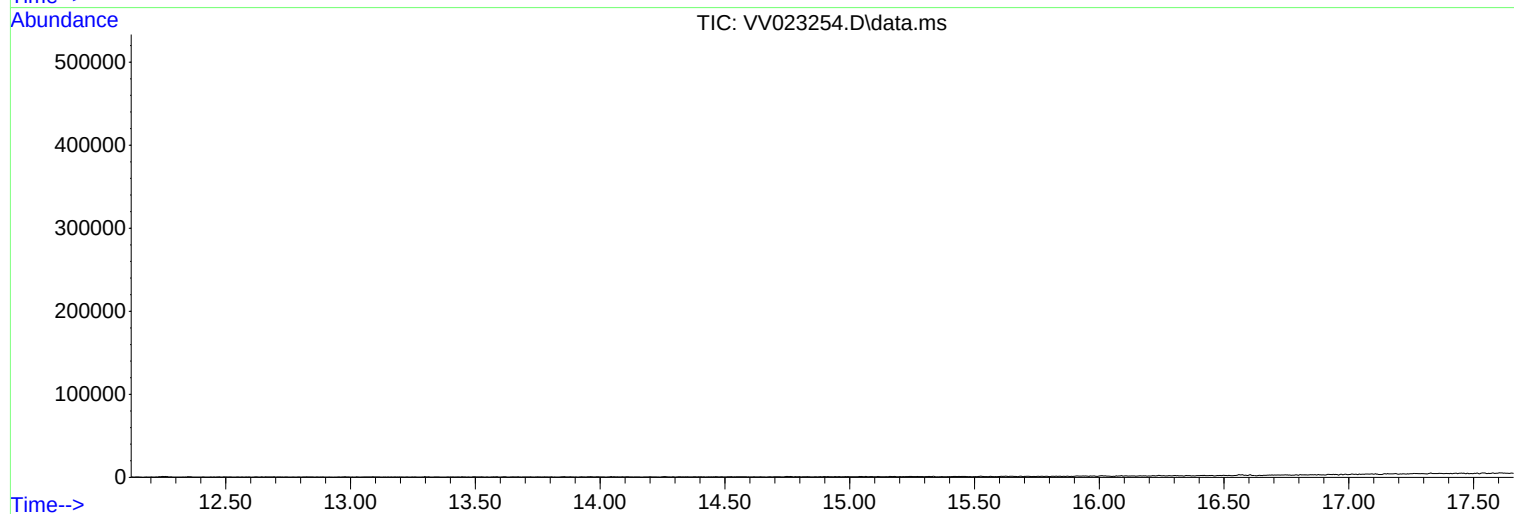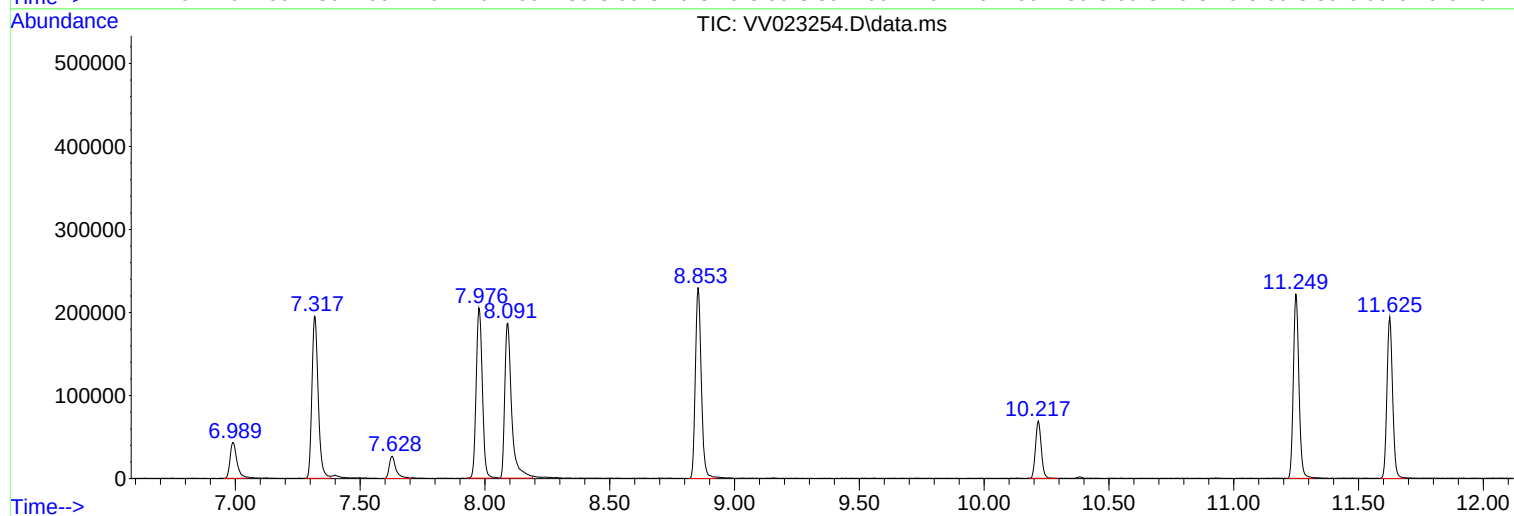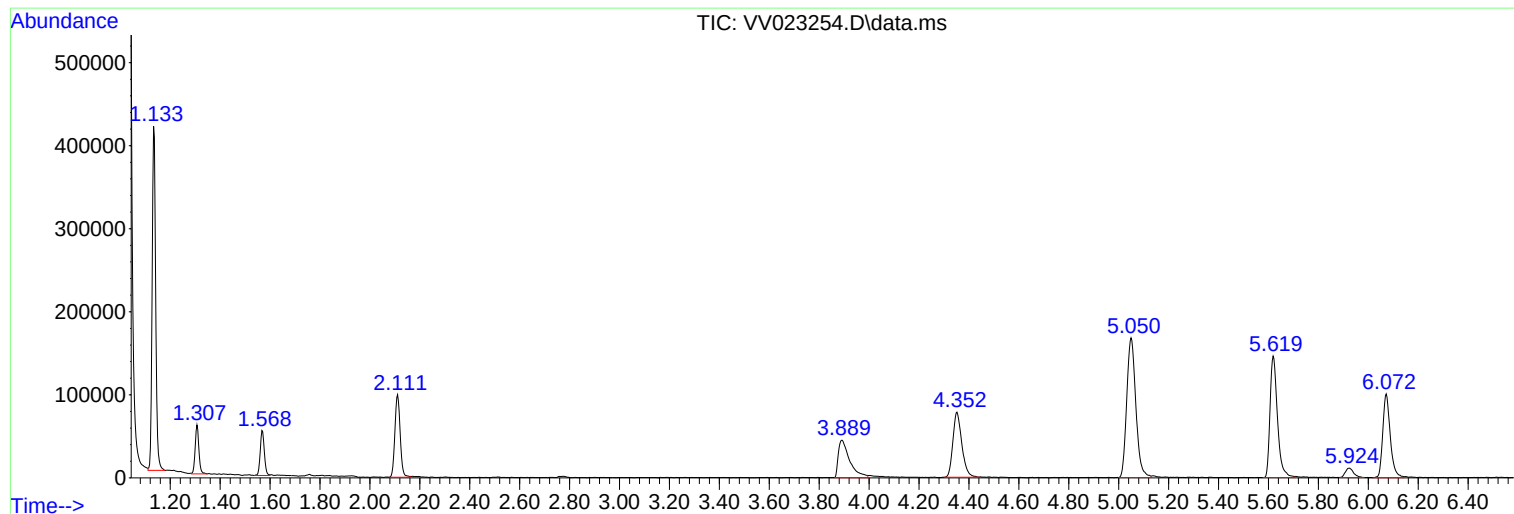

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023254.D
Acq On : 06 Nov 2021 00:11
Operator : SY/MD
Sample : M4535-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023254.D
Acq On : 06 Nov 2021 00:11
Operator : SY/MD
Sample : M4535-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4602

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc