

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023255.D
 Acq On : 06 Nov 2021 00:35
 Operator : SY/MD
 Sample : M4535-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4604

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	22	29	44	rVB	1077614	1064640	100.00%	18.170%
2	1.307	76	83	102	rVB	60102	66195	6.22%	1.130%
3	1.571	157	165	174	rBV	55106	64097	6.02%	1.094%
4	2.111	323	333	348	rBV	104072	153733	14.44%	2.624%
5	3.889	875	886	924	rBV2	49623	170053	15.97%	2.902%
6	4.352	1011	1030	1059	rBV	81051	215929	20.28%	3.685%
7	5.050	1229	1247	1274	rBV2	174938	446405	41.93%	7.619%
8	5.619	1413	1424	1446	rBV	145128	292180	27.44%	4.986%
9	5.918	1505	1517	1534	rBV2	57957	120760	11.34%	2.061%
10	6.072	1551	1565	1587	rBV	104119	214578	20.15%	3.662%
11	6.989	1838	1850	1873	rBV2	46147	88006	8.27%	1.502%
12	7.317	1940	1952	1974	rBV	203138	360208	33.83%	6.147%
13	7.625	2039	2048	2064	rBV	28021	50911	4.78%	0.869%
14	7.976	2142	2157	2183	rBV	612431	1032540	96.98%	17.622%
15	8.088	2183	2192	2224	rVV	206418	372727	35.01%	6.361%
16	8.853	2417	2430	2450	rBV	227411	375005	35.22%	6.400%
17	10.217	2841	2854	2869	rBV	72467	115307	10.83%	1.968%
18	11.249	3163	3175	3196	rBV	218048	340643	32.00%	5.814%
19	11.625	3280	3292	3311	rBV	198564	315519	29.64%	5.385%




Sum of corrected areas: 5859436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023255.D
Acq On : 06 Nov 2021 00:35
Operator : SY/MD
Sample : M4535-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

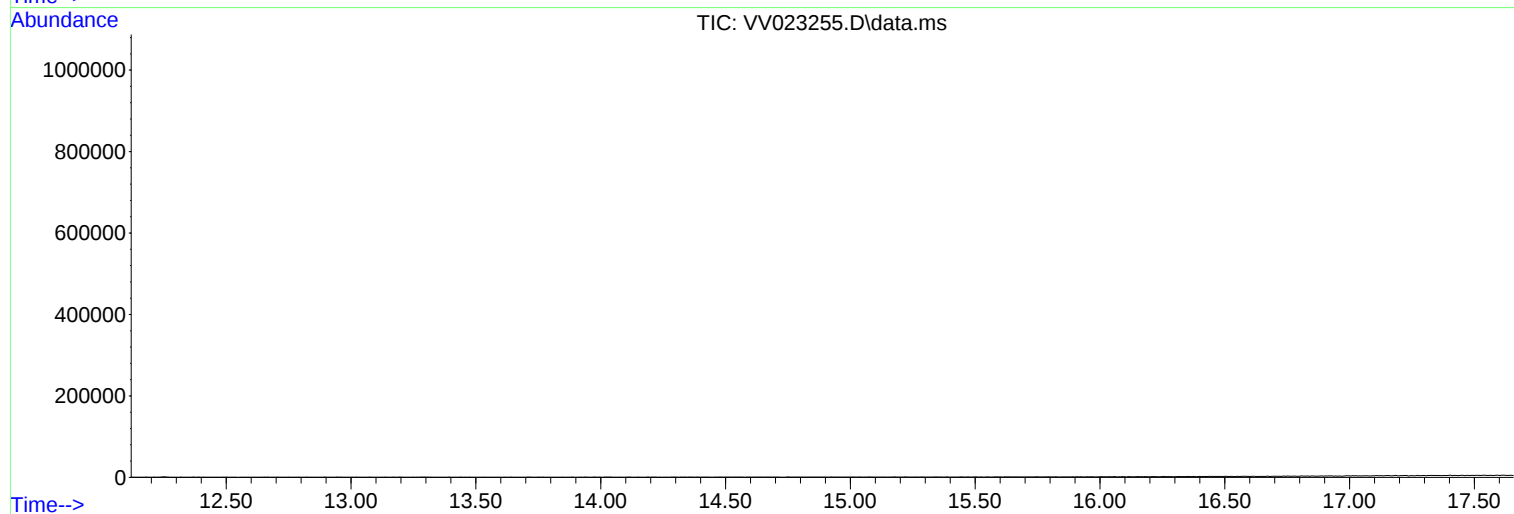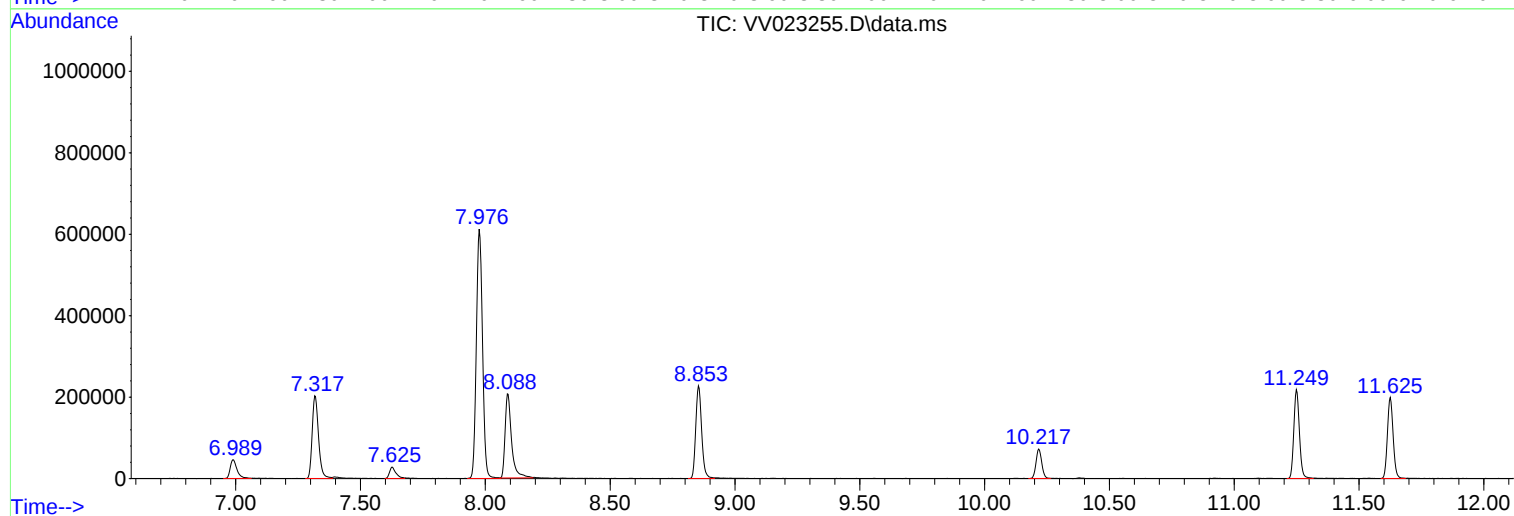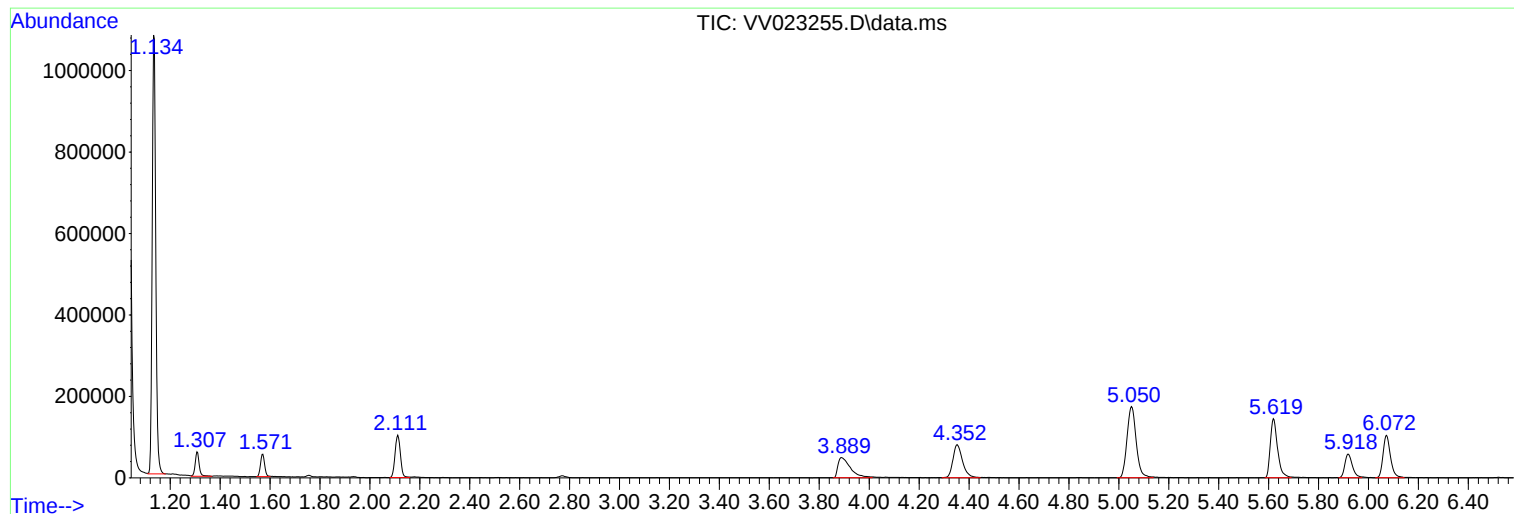

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023255.D
Acq On : 06 Nov 2021 00:35
Operator : SY/MD
Sample : M4535-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023255.D
Acq On : 06 Nov 2021 00:35
Operator : SY/MD
Sample : M4535-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4604

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
