

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023257.D
 Acq On : 06 Nov 2021 01:21
 Operator : SY/MD
 Sample : M4535-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4566

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	61455	63862	14.52%	1.754%
2	1.571	155	165	176	rBV	56090	64287	14.62%	1.766%
3	2.111	321	333	346	rBV	104248	151877	34.54%	4.173%
4	2.182	349	355	363	rVB2	2505	4695	1.07%	0.129%
5	3.892	876	887	918	rBV2	44810	144033	32.75%	3.957%
6	4.352	1012	1030	1056	rBV2	78255	198062	45.04%	5.441%
7	5.050	1231	1247	1271	rBV2	173133	439775	100.00%	12.082%
8	5.619	1413	1424	1448	rBV	146293	302050	68.68%	8.298%
9	5.912	1506	1515	1525	rBV6	3651	7114	1.62%	0.195%
10	6.072	1548	1565	1590	rBV	101477	211672	48.13%	5.815%
11	6.989	1839	1850	1870	rBV	44919	85838	19.52%	2.358%
12	7.320	1941	1953	1970	rBV	198387	353504	80.38%	9.712%
13	7.400	1974	1978	1998	rVB5	4212	8761	1.99%	0.241%
14	7.625	2040	2048	2068	rBV2	26682	50074	11.39%	1.376%
15	8.092	2182	2193	2229	rBV	186901	367238	83.51%	10.089%
16	8.854	2418	2430	2453	rBV	234855	383803	87.27%	10.544%
17	10.217	2841	2854	2870	rBV	69019	108431	24.66%	2.979%
18	11.249	3164	3175	3197	rBV	224526	349949	79.57%	9.614%
19	11.625	3281	3292	3311	rBV	199651	315540	71.75%	8.669%
20	12.252	3480	3487	3496	rVB2	7170	10892	2.48%	0.299%
21	14.043	4032	4044	4055	rVB	11829	18476	4.20%	0.508%




Sum of corrected areas: 3639933

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023257.D
Acq On : 06 Nov 2021 01:21
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

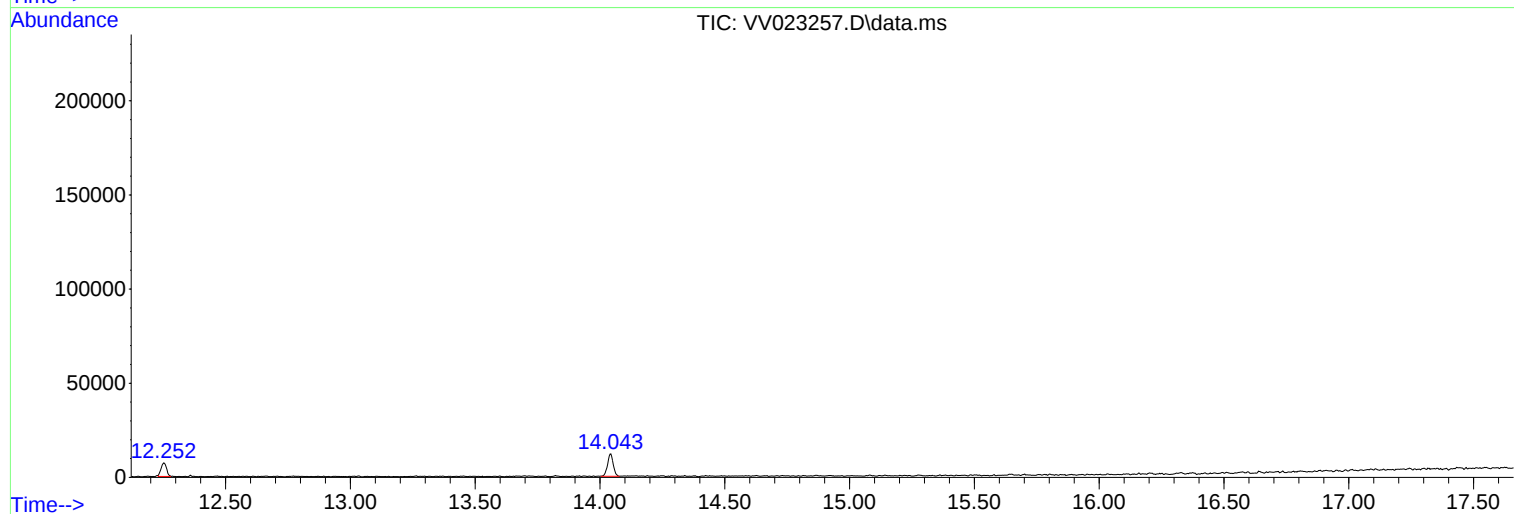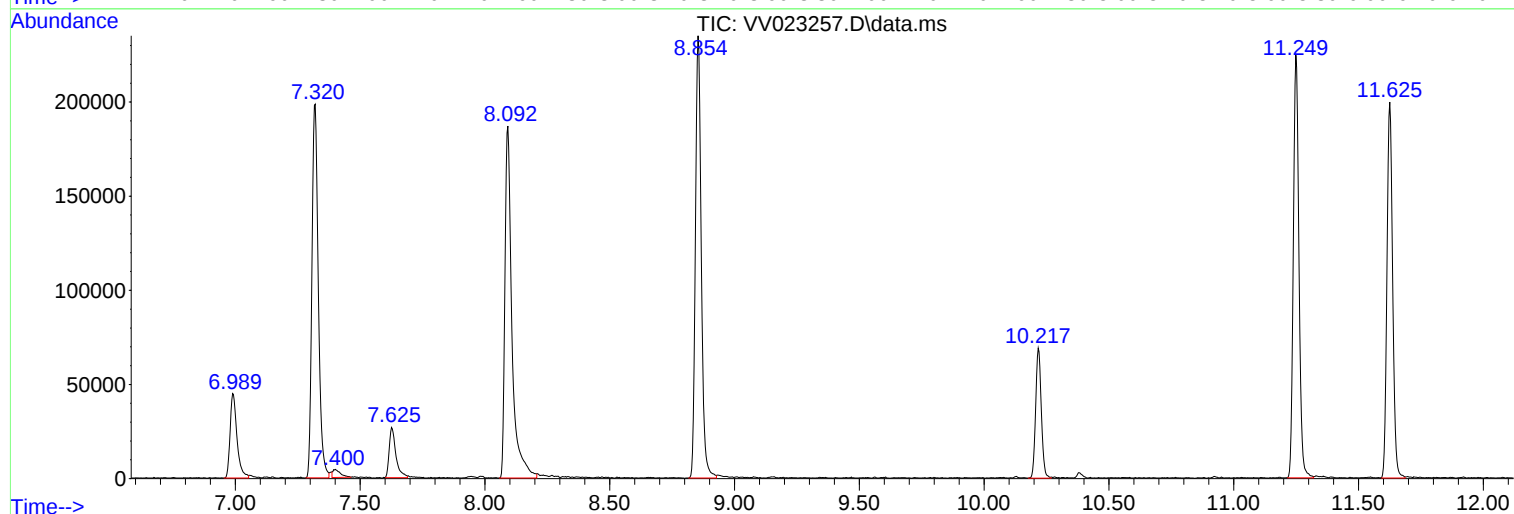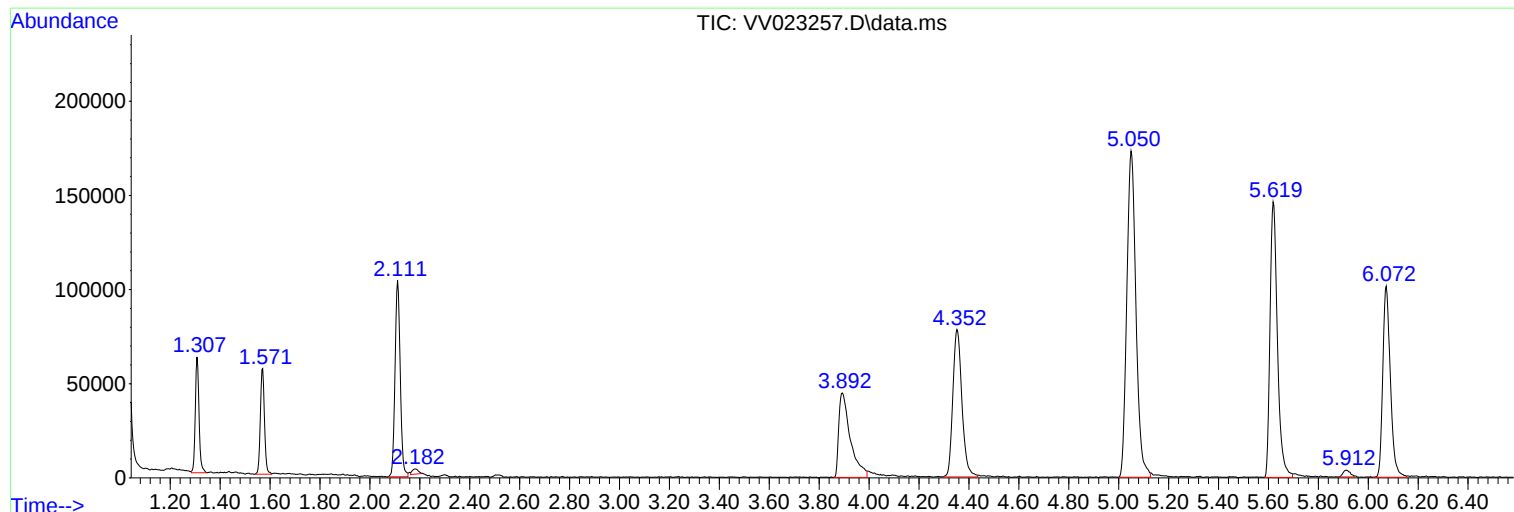

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023257.D
Acq On : 06 Nov 2021 01:21
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023257.D
Acq On : 06 Nov 2021 01:21
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc