

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023258.D
 Acq On : 06 Nov 2021 01:44
 Operator : SY/MD
 Sample : M4535-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4603

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	22	29	49	rVB	1155802	1120392	100.00%	21.236%
2	1.307	76	83	92	rVB	57569	59420	5.30%	1.126%
3	1.568	156	164	175	rBV	54824	61884	5.52%	1.173%
4	2.111	320	333	348	rBV	101795	148455	13.25%	2.814%
5	3.889	877	886	920	rBV	47085	159455	14.23%	3.022%
6	4.352	1012	1030	1059	rBV2	77085	205812	18.37%	3.901%
7	5.050	1231	1247	1275	rBV3	167072	424251	37.87%	8.041%
8	5.619	1411	1424	1451	rBV	160641	327618	29.24%	6.210%
9	5.918	1506	1517	1540	rBV3	46080	97397	8.69%	1.846%
10	6.072	1553	1565	1584	rBV	101249	206745	18.45%	3.919%
11	6.989	1837	1850	1868	rBV2	44206	83884	7.49%	1.590%
12	7.317	1940	1952	1973	rBV	195186	344001	30.70%	6.520%
13	7.625	2038	2048	2068	rBV2	26544	50661	4.52%	0.960%
14	7.976	2139	2157	2175	rBV	253155	419659	37.46%	7.954%
15	8.088	2182	2192	2225	rBV	189192	362190	32.33%	6.865%
16	8.854	2419	2430	2448	rBV	258456	414861	37.03%	7.863%
17	10.217	2842	2854	2868	rBV	70824	110872	9.90%	2.102%
18	11.249	3164	3175	3197	rBV	247818	375746	33.54%	7.122%
19	11.625	3280	3292	3308	rBV	193165	302506	27.00%	5.734%




Sum of corrected areas: 5275809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023258.D
Acq On : 06 Nov 2021 01:44
Operator : SY/MD
Sample : M4535-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4603

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

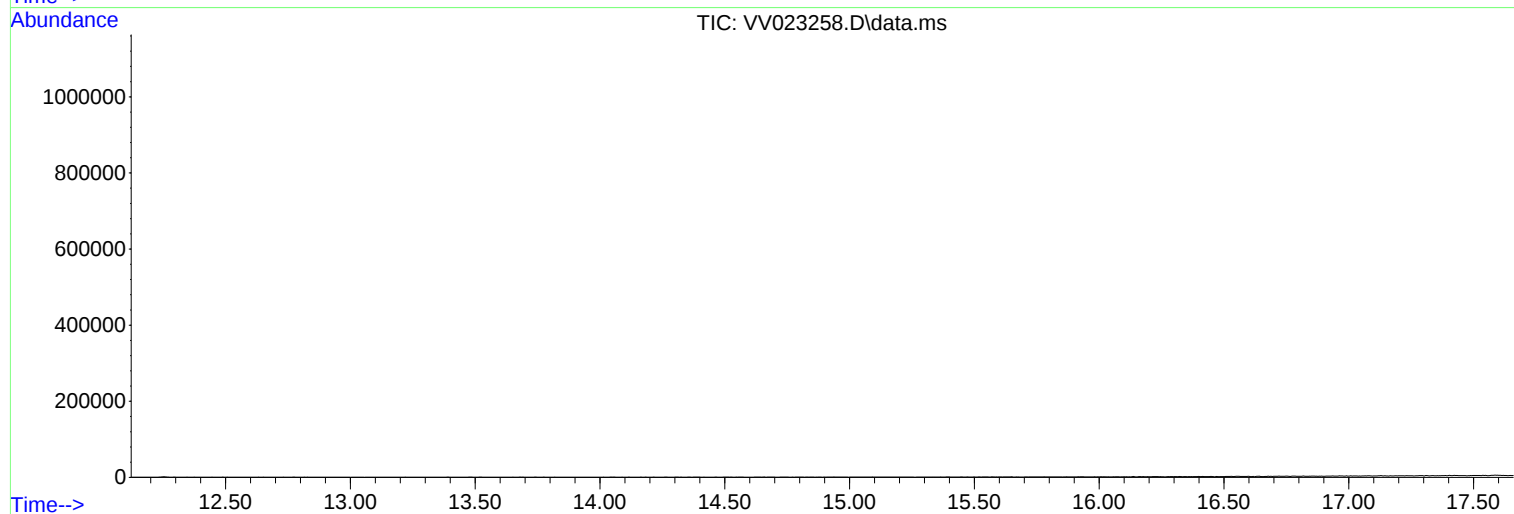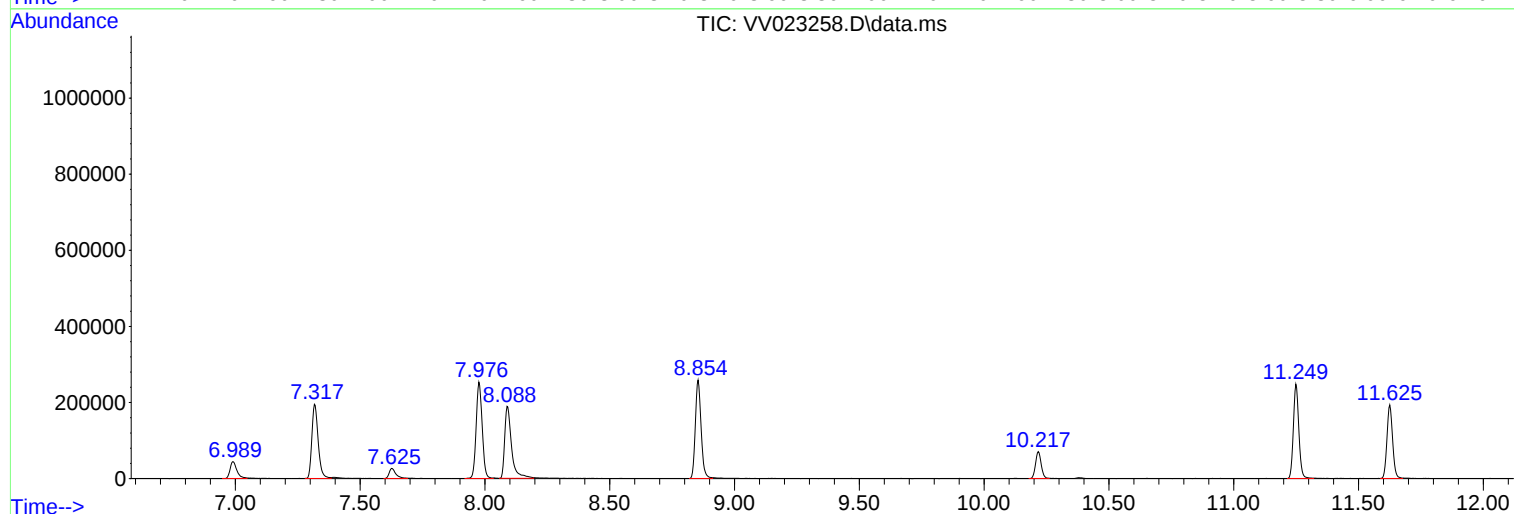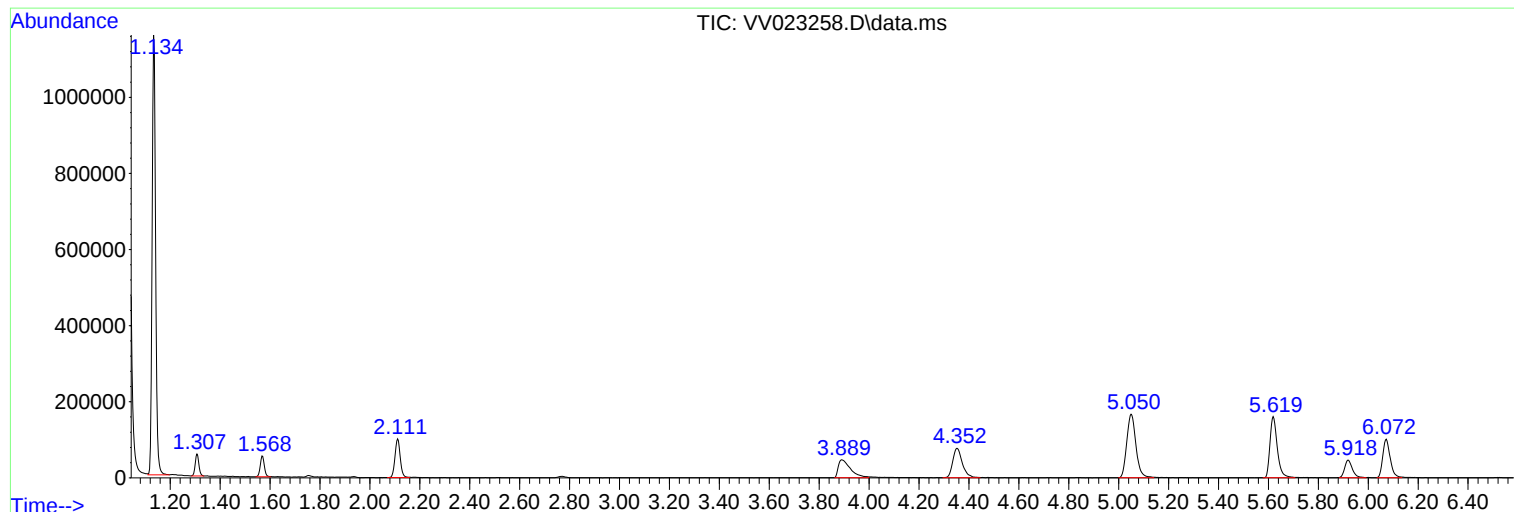

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023258.D
Acq On : 06 Nov 2021 01:44
Operator : SY/MD
Sample : M4535-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4603

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023258.D
Acq On : 06 Nov 2021 01:44
Operator : SY/MD
Sample : M4535-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4603

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc