

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023262.D
 Acq On : 06 Nov 2021 03:17
 Operator : SY/MD
 Sample : M4534-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB859

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	66625	72376	15.69%	1.865%
2	1.571	157	165	175	rBV	58135	66264	14.36%	1.708%
3	2.111	322	333	347	rBV	108880	157063	34.04%	4.047%
4	3.892	877	887	924	rBV	47814	160220	34.72%	4.129%
5	4.352	1015	1030	1056	rBV2	80907	206445	44.74%	5.320%
6	5.050	1232	1247	1275	rBV2	186145	461425	100.00%	11.890%
7	5.619	1412	1424	1452	rBV	161291	330116	71.54%	8.506%
8	5.918	1509	1517	1527	rBV	2434	5069	1.10%	0.131%
9	6.072	1552	1565	1586	rBV2	105766	220341	47.75%	5.678%
10	6.989	1839	1850	1866	rBV	47587	91495	19.83%	2.358%
11	7.317	1938	1952	1970	rBV	216150	380838	82.54%	9.813%
12	7.400	1970	1978	1992	rVB3	8201	16628	3.60%	0.428%
13	7.625	2036	2048	2069	rBV2	29133	54050	11.71%	1.393%
14	8.092	2180	2193	2220	rBV	207888	389941	84.51%	10.048%
15	8.854	2416	2430	2449	rBV	250149	409730	88.80%	10.558%
16	9.143	2513	2520	2530	rBV5	4822	7802	1.69%	0.201%
17	10.217	2842	2854	2869	rBV	74964	118914	25.77%	3.064%
18	10.381	2896	2905	2915	rVB3	4238	6859	1.49%	0.177%
19	10.921	3065	3073	3082	rBV5	3168	4774	1.03%	0.123%
20	11.249	3164	3175	3191	rBV	248405	383993	83.22%	9.895%
21	11.625	3281	3292	3309	rBV	210222	336418	72.91%	8.669%




Sum of corrected areas: 3880761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023262.D
Acq On : 06 Nov 2021 03:17
Operator : SY/MD
Sample : M4534-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB859

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

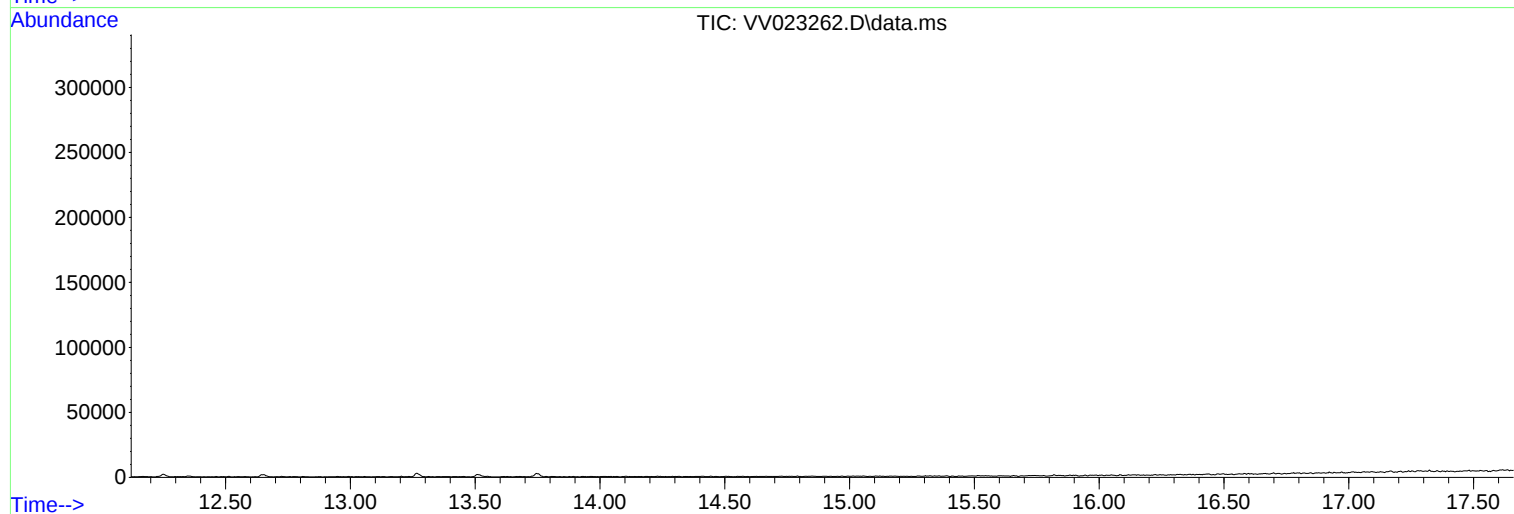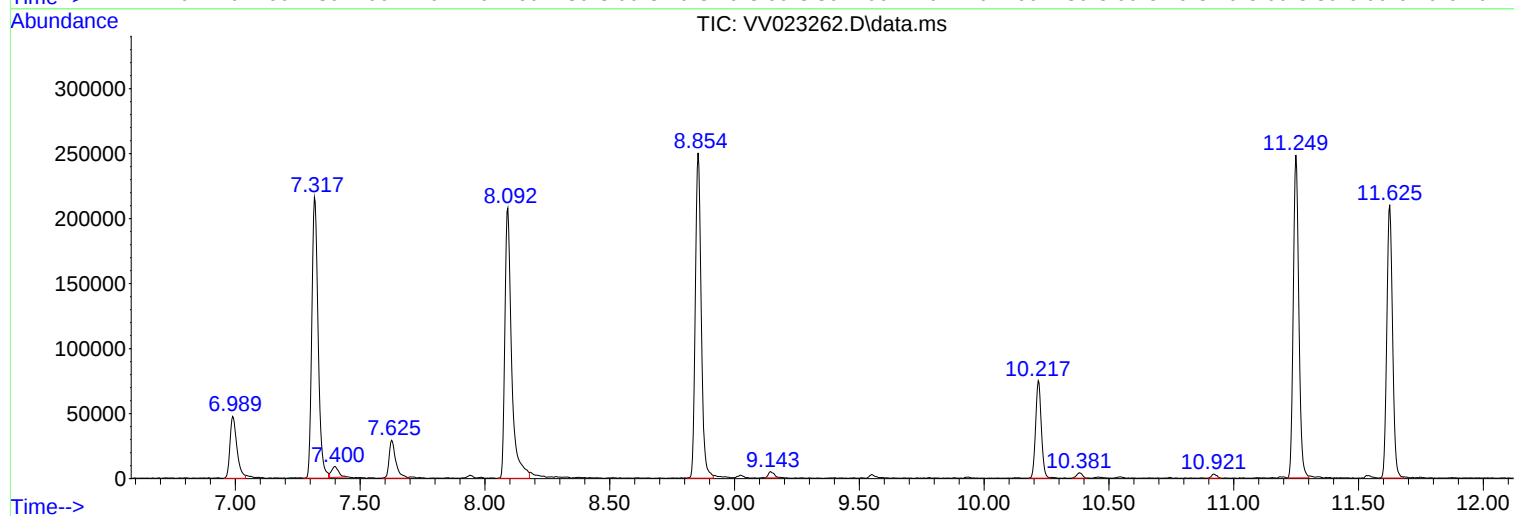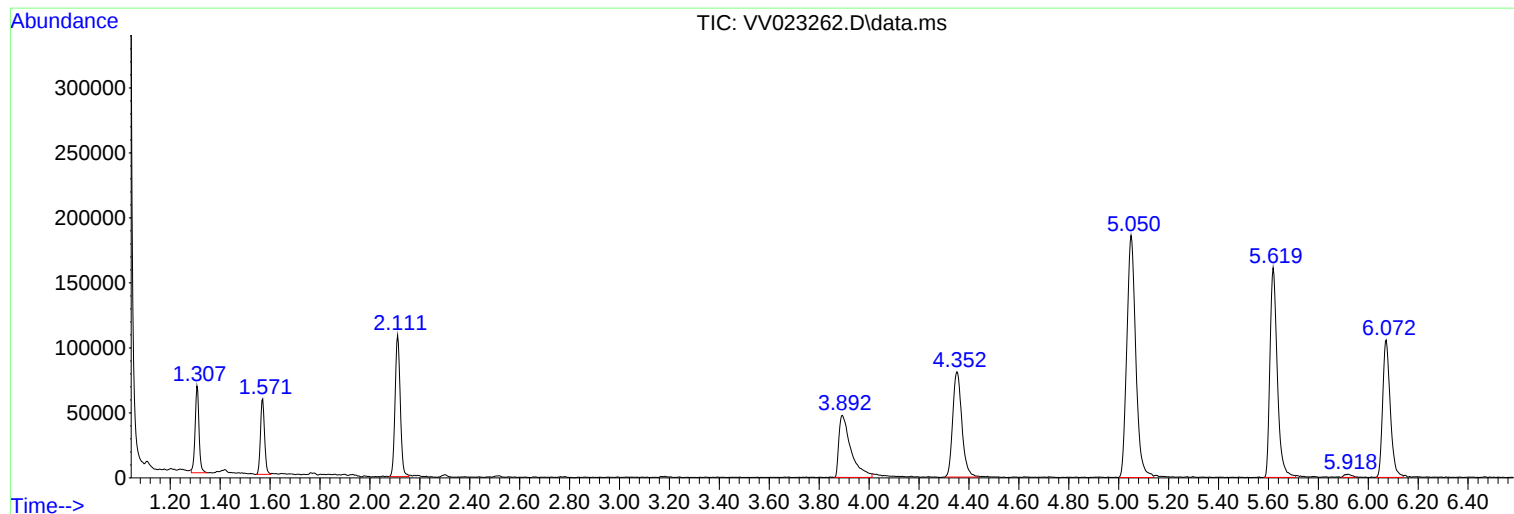

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023262.D
Acq On : 06 Nov 2021 03:17
Operator : SY/MD
Sample : M4534-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB859

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023262.D
Acq On : 06 Nov 2021 03:17
Operator : SY/MD
Sample : M4534-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB859

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc