

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023263.D
 Acq On : 06 Nov 2021 03:41
 Operator : SY/MD
 Sample : M4534-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB860

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	19	21	32	rVB2	9498	9759	2.12%	0.246%
2	1.307	76	83	96	rVB	64654	68258	14.83%	1.720%
3	1.571	157	165	177	rBV	58151	65867	14.31%	1.660%
4	2.111	322	333	351	rBV	105853	155127	33.70%	3.909%
5	3.892	877	887	921	rBV	48274	156695	34.04%	3.948%
6	4.352	1012	1030	1052	rBV	81440	204619	44.45%	5.156%
7	5.050	1232	1247	1273	rBV4	179920	457700	99.42%	11.532%
8	5.619	1412	1424	1451	rBV	161922	332060	72.13%	8.367%
9	6.072	1549	1565	1584	rBV	104158	219632	47.71%	5.534%
10	6.989	1837	1850	1874	rBV	48015	90917	19.75%	2.291%
11	7.317	1941	1952	1969	rBV	211224	371072	80.60%	9.350%
12	7.628	2039	2049	2068	rBV2	28187	53564	11.63%	1.350%
13	8.091	2183	2193	2229	rBV	206278	389863	84.68%	9.823%
14	8.854	2419	2430	2435	rBV	270908	428509	93.08%	10.797%
15	10.217	2841	2854	2872	rBV	74467	117824	25.59%	2.969%
16	11.188	3148	3156	3165	rBV4	5259	7625	1.66%	0.192%
17	11.249	3165	3175	3199	rBV2	255231	460383	100.00%	11.600%
18	11.625	3281	3292	3306	rBV	214183	341210	74.11%	8.597%
19	15.503	4488	4498	4509	rBV3	8978	13480	2.93%	0.340%
20	16.310	4740	4749	4758	rBV2	17172	24650	5.35%	0.621%




Sum of corrected areas: 3968814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023263.D
Acq On : 06 Nov 2021 03:41
Operator : SY/MD
Sample : M4534-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB860

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

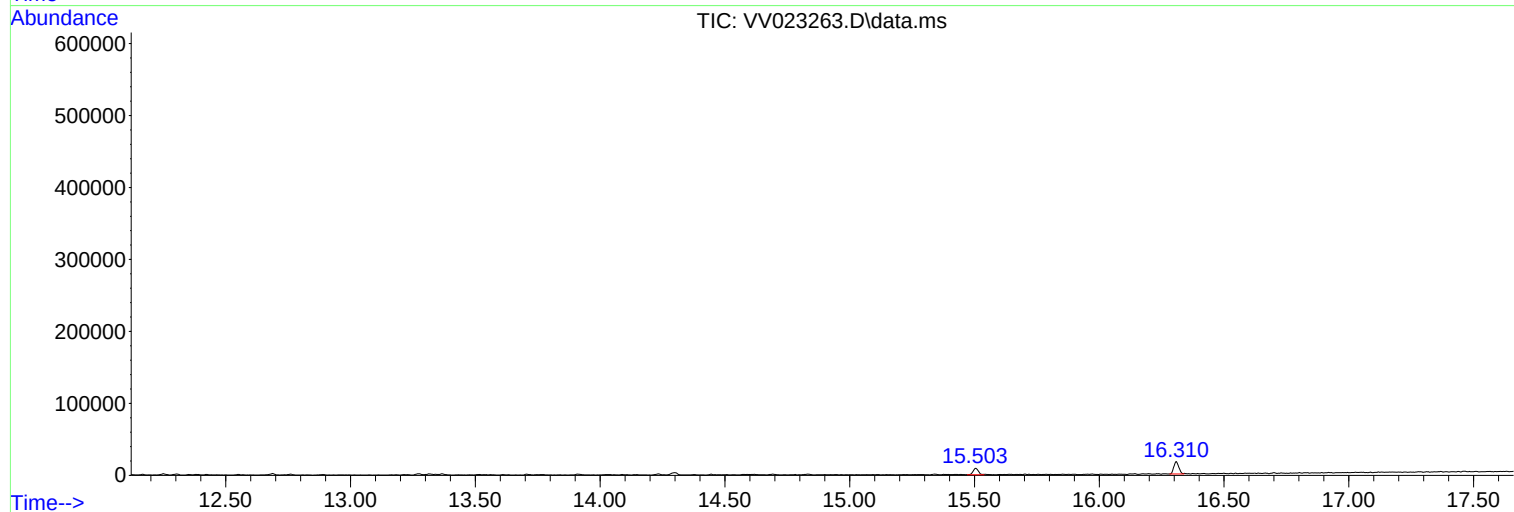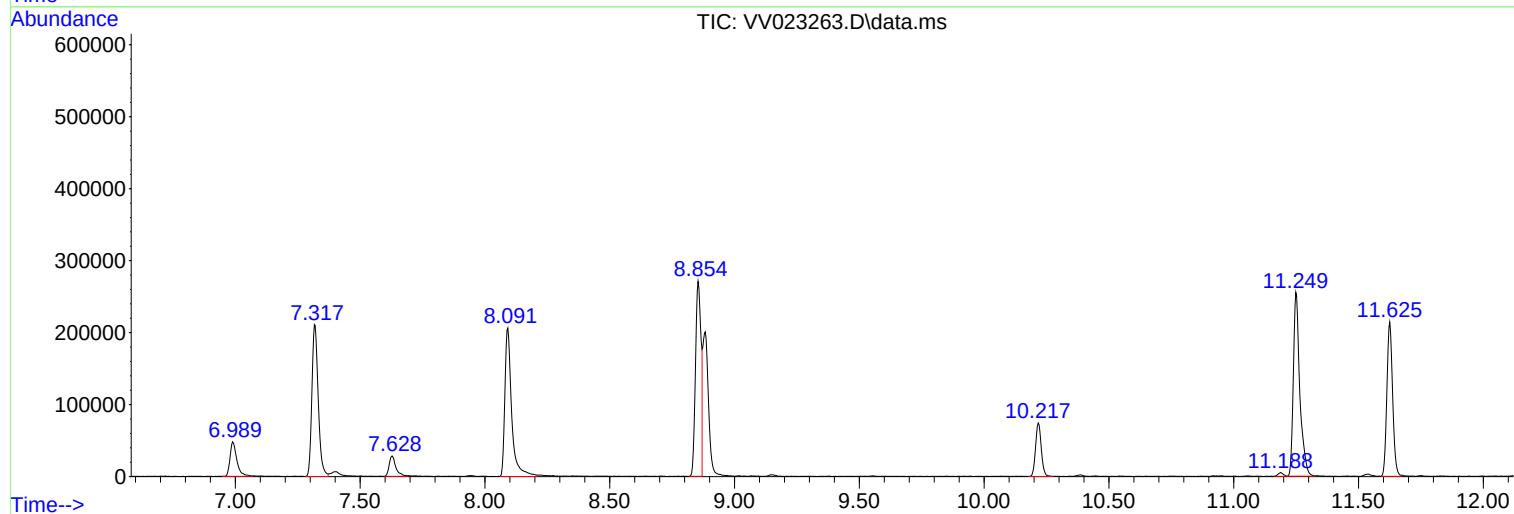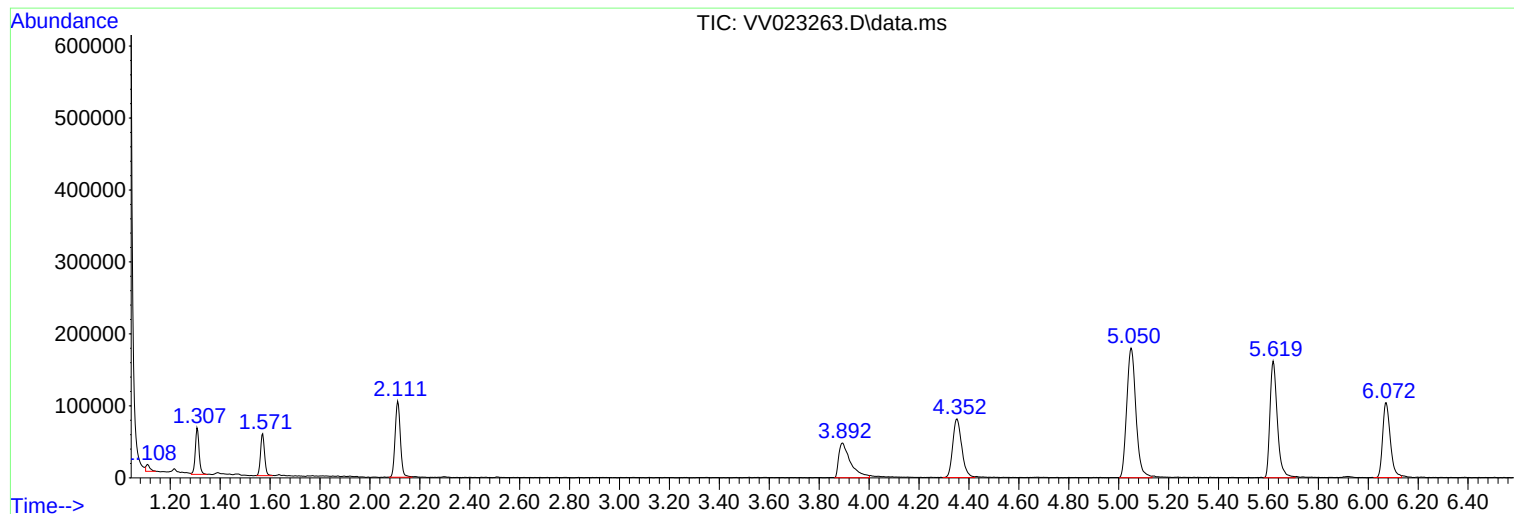

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023263.D
Acq On : 06 Nov 2021 03:41
Operator : SY/MD
Sample : M4534-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB860

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023263.D
Acq On : 06 Nov 2021 03:41
Operator : SY/MD
Sample : M4534-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB860

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc