

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023265.D
 Acq On : 06 Nov 2021 04:27
 Operator : SY/MD
 Sample : M4545-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4605

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	23	29	43	rVB	187715	186804	42.87%	4.381%
2	1.307	76	83	93	rVB	61089	64421	14.78%	1.511%
3	1.571	157	165	174	rBV	57187	63816	14.64%	1.497%
4	2.111	319	333	345	rBV	103174	152010	34.88%	3.565%
5	2.301	383	392	402	rBV2	3251	5467	1.25%	0.128%
6	2.773	530	539	552	rVB4	2783	5713	1.31%	0.134%
7	3.892	877	887	920	rBV2	46677	160232	36.77%	3.758%
8	4.352	1014	1030	1057	rBV	79726	204209	46.86%	4.789%
9	5.050	1229	1247	1271	rBV2	172631	435791	100.00%	10.221%
10	5.619	1413	1424	1445	rBV	152812	309657	71.06%	7.263%
11	5.921	1507	1518	1533	rBV3	25177	52335	12.01%	1.227%
12	6.072	1552	1565	1586	rBV2	99993	207975	47.72%	4.878%
13	6.989	1838	1850	1874	rBV	45010	85343	19.58%	2.002%
14	7.317	1941	1952	1971	rBV	200567	354168	81.27%	8.307%
15	7.625	2040	2048	2066	rBV2	27041	49156	11.28%	1.153%
16	7.979	2139	2158	2180	rBV	202578	345984	79.39%	8.115%
17	8.092	2183	2193	2231	rVV	200973	374575	85.95%	8.785%
18	8.854	2419	2430	2449	rBV	241534	393299	90.25%	9.224%
19	10.217	2843	2854	2866	rBV	72645	113532	26.05%	2.663%
20	11.249	3164	3175	3194	rBV	236689	366150	84.02%	8.588%
21	11.535	3252	3264	3279	rBV3	7674	14346	3.29%	0.336%
22	11.625	3281	3292	3311	rVV	204255	318729	73.14%	7.475%




Sum of corrected areas: 4263712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023265.D
Acq On : 06 Nov 2021 04:27
Operator : SY/MD
Sample : M4545-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

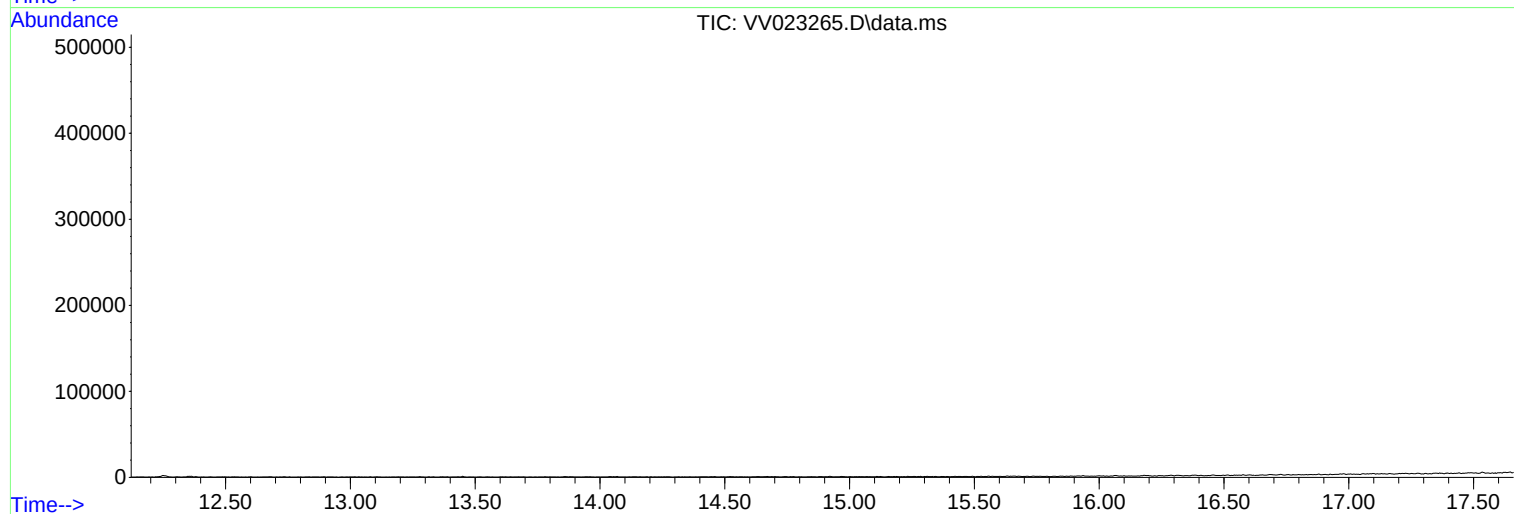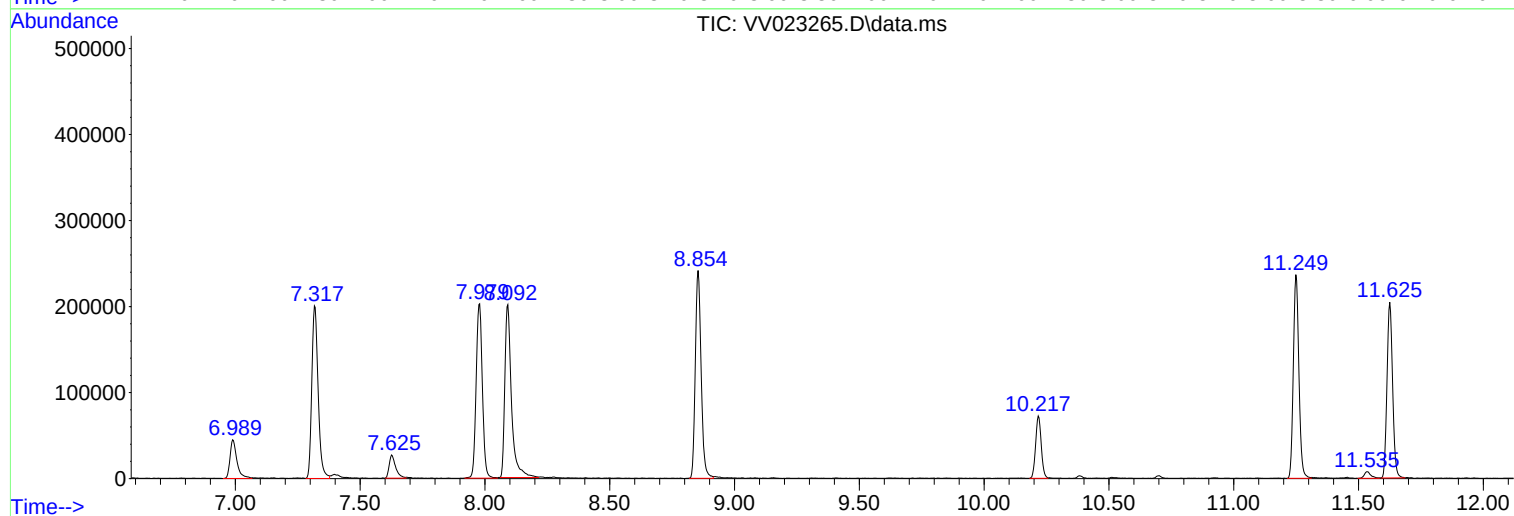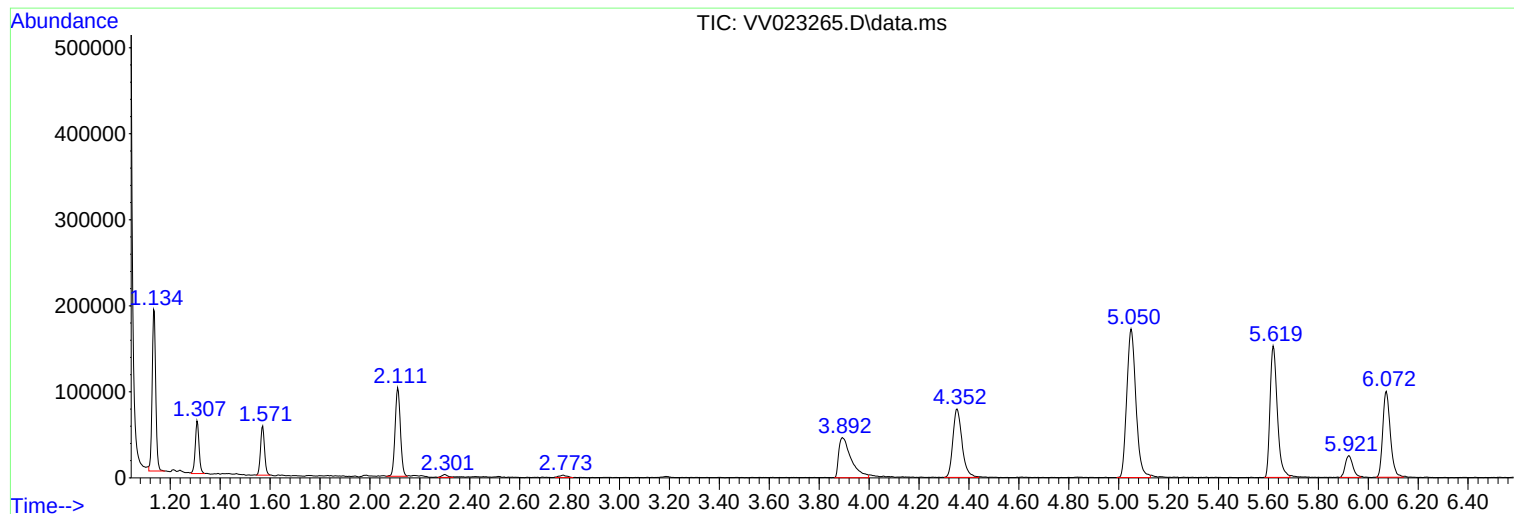

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023265.D
Acq On : 06 Nov 2021 04:27
Operator : SY/MD
Sample : M4545-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023265.D
Acq On : 06 Nov 2021 04:27
Operator : SY/MD
Sample : M4545-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4605

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc