

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023268.D
 Acq On : 06 Nov 2021 05:37
 Operator : SY/MD
 Sample : M4545-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4606

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	60136	61471	13.34%	1.579%
2	1.571	156	165	175	rBV	58886	66956	14.53%	1.719%
3	2.114	323	334	349	rVB3	121256	195166	42.35%	5.012%
4	3.896	877	888	930	rBV	45309	159605	34.63%	4.098%
5	4.352	1014	1030	1053	rBV	81221	204882	44.46%	5.261%
6	4.616	1098	1112	1128	rVB3	6957	16439	3.57%	0.422%
7	5.050	1232	1247	1277	rBV2	182954	460835	100.00%	11.834%
8	5.619	1413	1424	1448	rBV	157213	321875	69.85%	8.265%
9	5.918	1508	1517	1526	rBV7	2723	5478	1.19%	0.141%
10	6.072	1553	1565	1591	rBV	104482	218899	47.50%	5.621%
11	6.989	1840	1850	1870	rBV2	47497	90459	19.63%	2.323%
12	7.317	1938	1952	1971	rBV	214205	378035	82.03%	9.708%
13	7.625	2039	2048	2064	rBV2	28591	52305	11.35%	1.343%
14	7.979	2149	2158	2172	rVB3	16899	30413	6.60%	0.781%
15	8.092	2183	2193	2226	rBV	211972	397759	86.31%	10.214%
16	8.854	2418	2430	2460	rBV	247658	404568	87.79%	10.389%
17	10.217	2839	2854	2868	rBV	74930	117978	25.60%	3.030%
18	11.249	3164	3175	3195	rBV	240884	374277	81.22%	9.611%
19	11.625	3280	3292	3313	rBV	209697	336834	73.09%	8.650%




Sum of corrected areas: 3894234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023268.D
Acq On : 06 Nov 2021 05:37
Operator : SY/MD
Sample : M4545-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4606

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

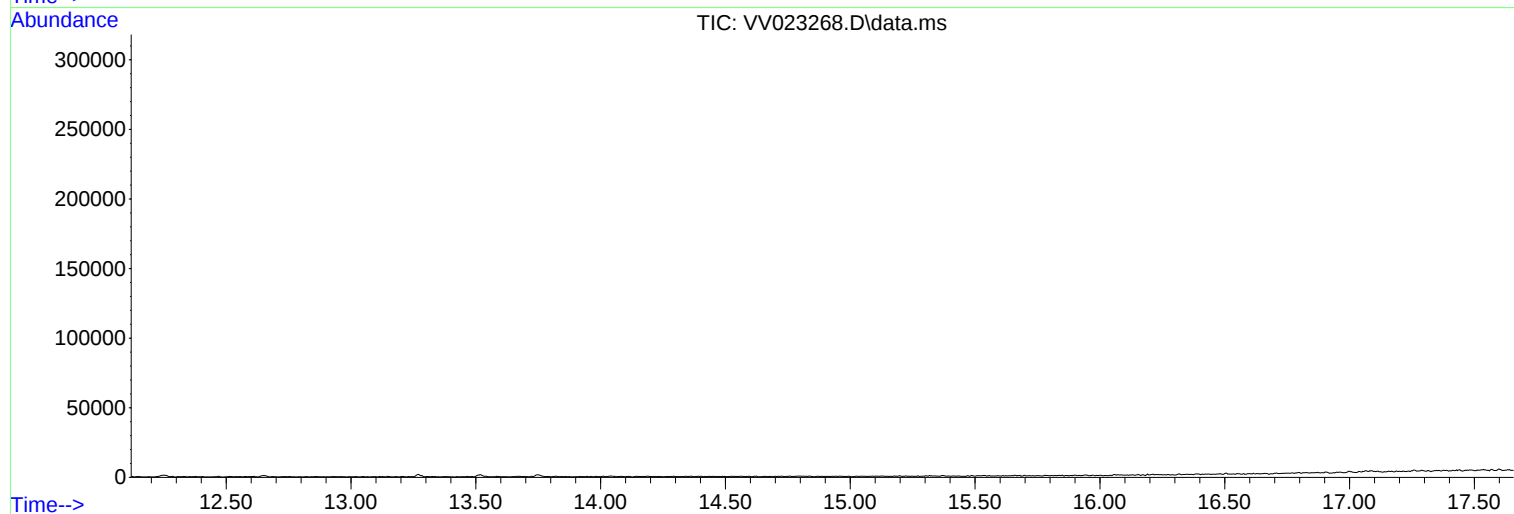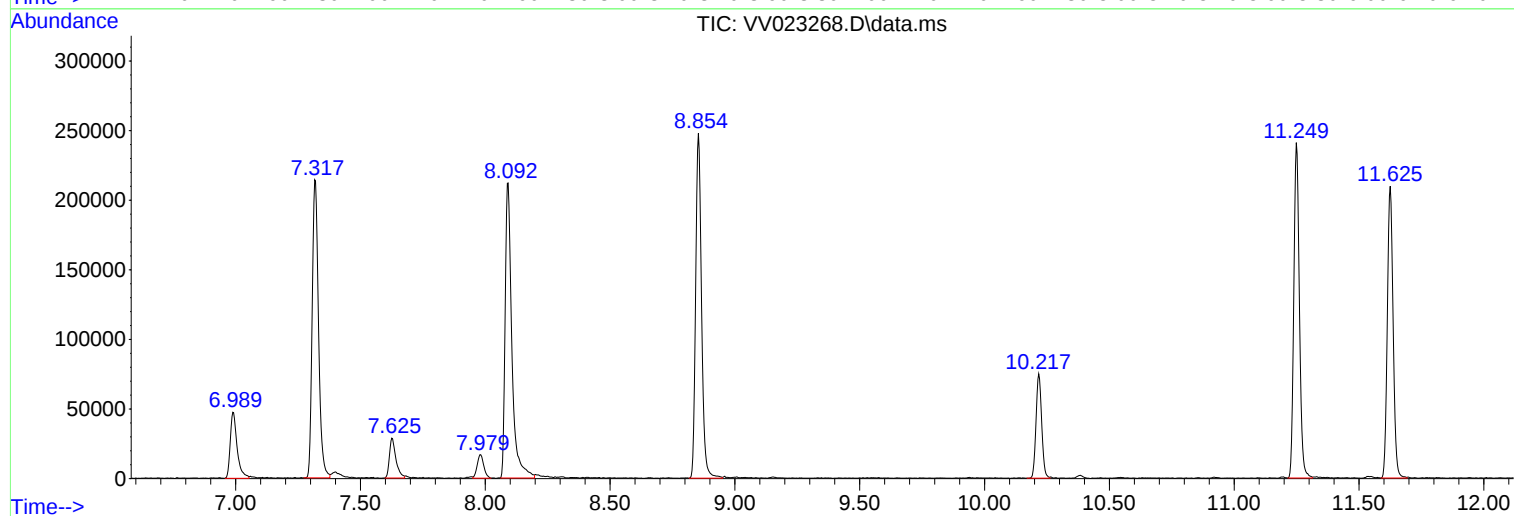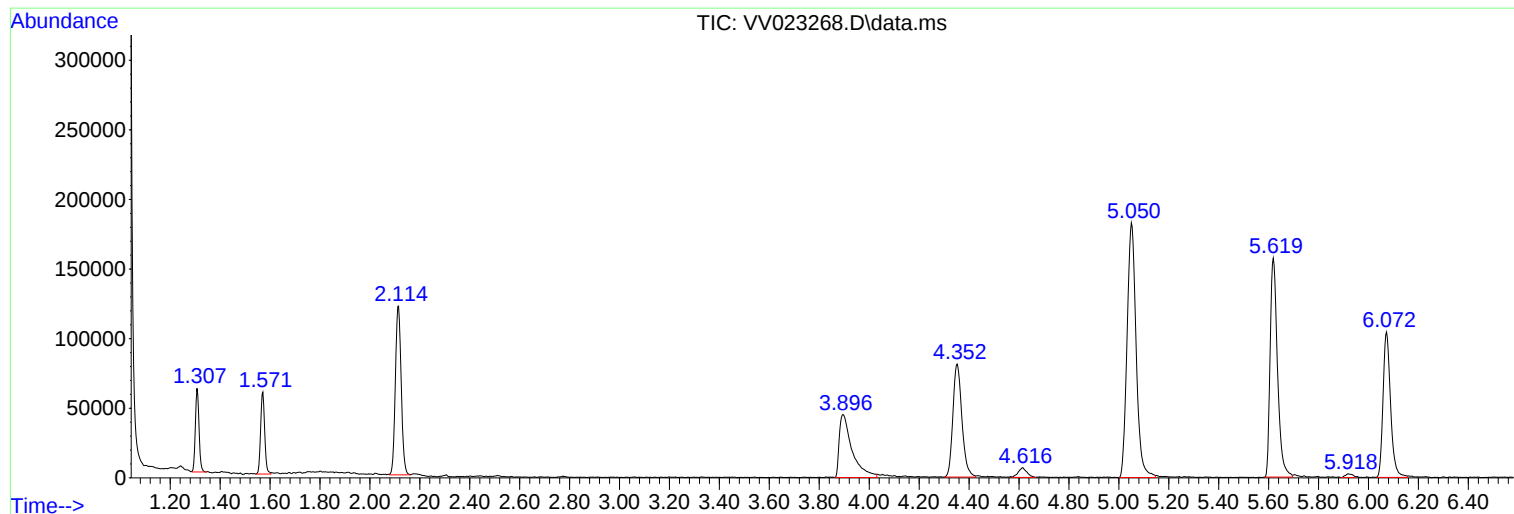

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023268.D
Acq On : 06 Nov 2021 05:37
Operator : SY/MD
Sample : M4545-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4606

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023268.D
Acq On : 06 Nov 2021 05:37
Operator : SY/MD
Sample : M4545-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4606

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc