

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023269.D
 Acq On : 06 Nov 2021 06:00
 Operator : SY/MD
 Sample : M4545-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4612

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	56756	58216	13.60%	1.467%
2	1.571	154	165	176	rBV	55268	63154	14.75%	1.591%
3	2.111	323	333	348	rBV	99234	144295	33.71%	3.636%
4	3.892	877	887	916	rBV	41801	137995	32.24%	3.477%
5	4.352	1014	1030	1058	rBV	77133	197784	46.20%	4.983%
6	5.050	1231	1247	1276	rBV2	168190	428072	100.00%	10.786%
7	5.619	1412	1424	1453	rBV	153748	313582	73.25%	7.901%
8	5.924	1508	1519	1536	rBV6	8590	18076	4.22%	0.455%
9	6.072	1552	1565	1585	rBV2	100699	205326	47.97%	5.173%
10	6.989	1841	1850	1870	rBV	43461	83988	19.62%	2.116%
11	7.317	1941	1952	1972	rBV	196445	347508	81.18%	8.756%
12	7.403	1972	1979	1992	rVB7	3542	7949	1.86%	0.200%
13	7.625	2040	2048	2064	rBV2	25972	47342	11.06%	1.193%
14	7.976	2144	2157	2173	rBV	225957	371750	86.84%	9.367%
15	8.091	2182	2193	2227	rBV	198186	367502	85.85%	9.260%
16	8.854	2419	2430	2454	rBV	239722	391067	91.36%	9.853%
17	10.217	2842	2854	2875	rBV	70658	112081	26.18%	2.824%
18	11.249	3164	3175	3196	rBV	234180	362539	84.69%	9.135%
19	11.625	3280	3292	3310	rBV	199019	310646	72.57%	7.827%




Sum of corrected areas: 3968872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023269.D
Acq On : 06 Nov 2021 06:00
Operator : SY/MD
Sample : M4545-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

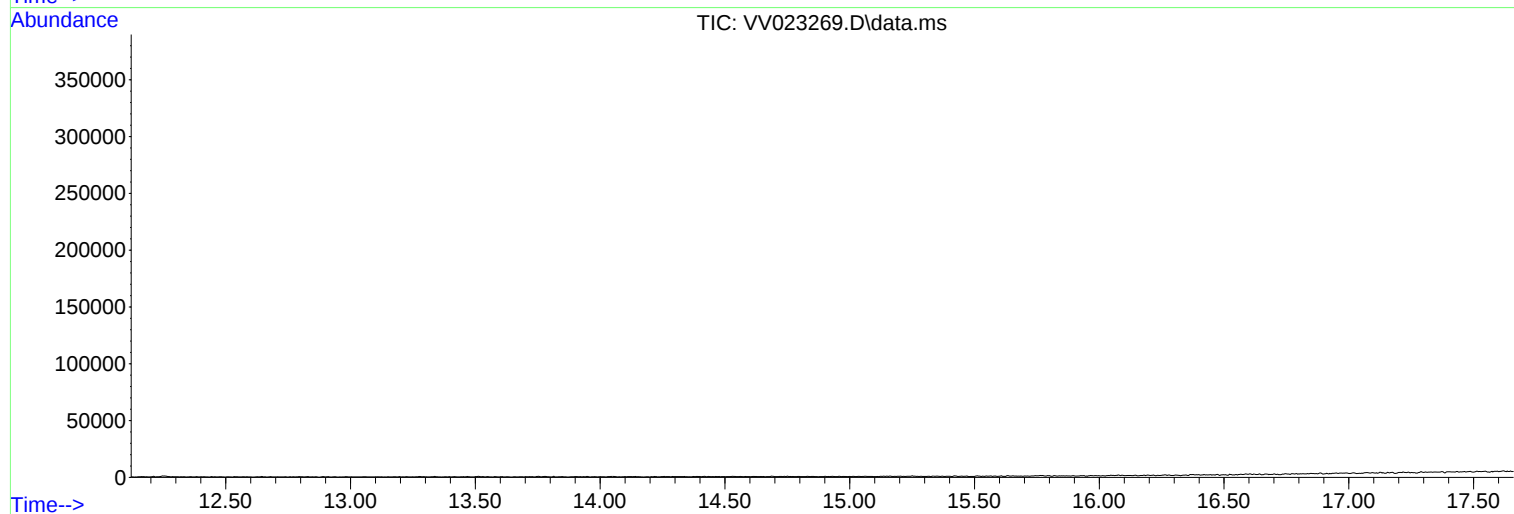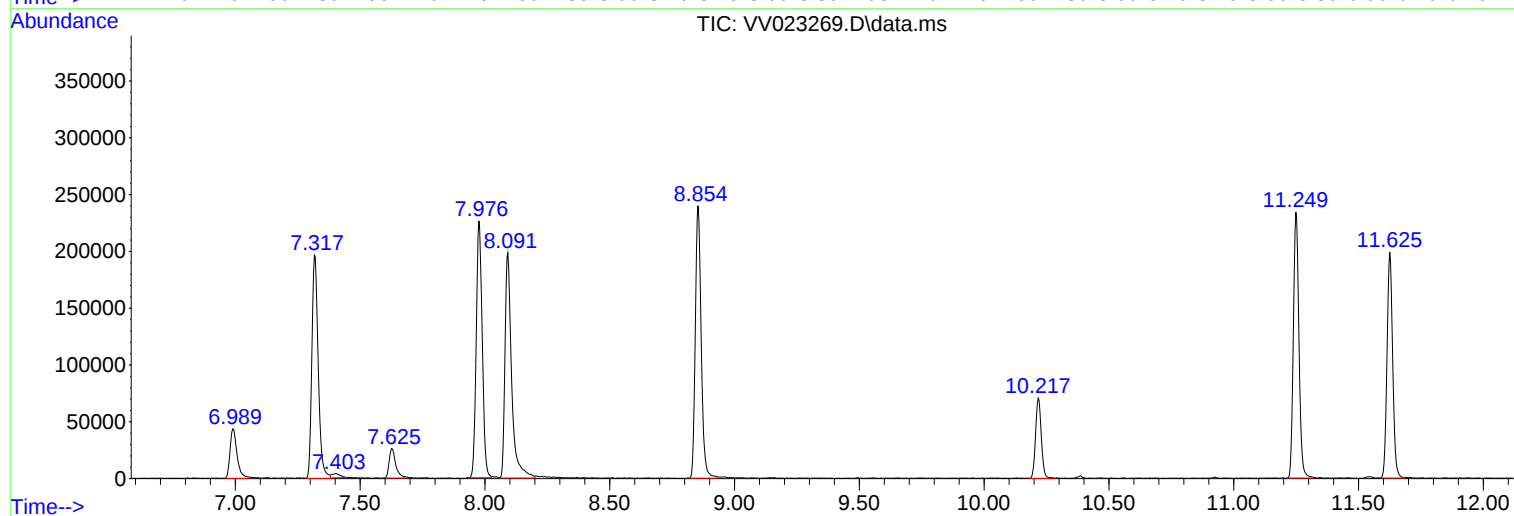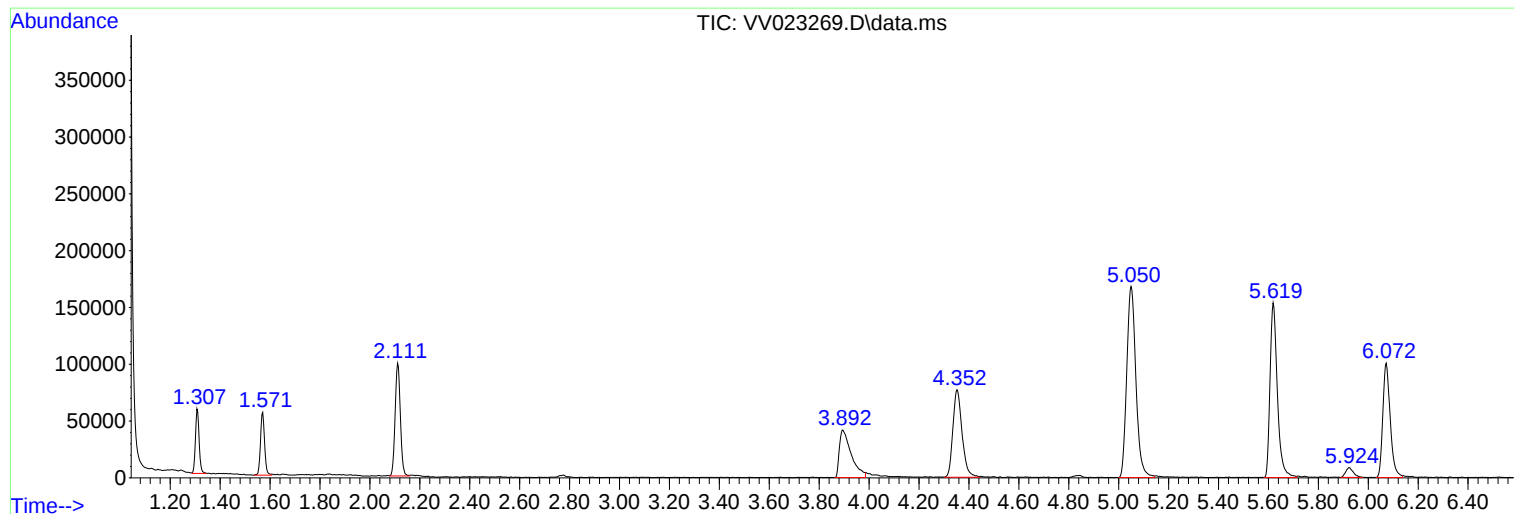

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023269.D
Acq On : 06 Nov 2021 06:00
Operator : SY/MD
Sample : M4545-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023269.D
Acq On : 06 Nov 2021 06:00
Operator : SY/MD
Sample : M4545-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc