

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
 Data File : VV023270.D
 Acq On : 06 Nov 2021 06:23
 Operator : SY/MD
 Sample : M4545-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4613

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	59646	63248	8.65%	1.389%
2	1.571	156	165	177	rBV	57421	66058	9.03%	1.451%
3	2.111	321	333	348	rBV	102422	149707	20.47%	3.288%
4	2.774	525	539	551	rBV3	5553	11986	1.64%	0.263%
5	3.896	875	888	917	rBV2	46423	160110	21.89%	3.516%
6	4.352	1009	1030	1054	rBV	81970	213312	29.17%	4.685%
7	5.050	1228	1247	1271	rBV2	177347	446784	61.09%	9.812%
8	5.619	1413	1424	1445	rBV	157997	322254	44.06%	7.077%
9	5.921	1507	1518	1541	rBV4	42296	89272	12.21%	1.961%
10	6.072	1552	1565	1589	rBV	104800	215929	29.52%	4.742%
11	6.989	1839	1850	1873	rBV	46010	88738	12.13%	1.949%
12	7.317	1941	1952	1971	rBV	205770	362924	49.62%	7.971%
13	7.629	2039	2049	2075	rBV2	27734	51869	7.09%	1.139%
14	7.976	2145	2157	2177	rBV	441865	731394	100.00%	16.063%
15	8.088	2183	2192	2228	rVB	197558	364358	49.82%	8.002%
16	8.854	2417	2430	2455	rBV	246996	405704	55.47%	8.910%
17	10.217	2843	2854	2874	rVB	73243	115638	15.81%	2.540%
18	11.249	3158	3175	3197	rBV	235008	373061	51.01%	8.193%
19	11.625	3280	3292	3307	rBV	202851	320954	43.88%	7.049%




Sum of corrected areas: 4553300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023270.D
Acq On : 06 Nov 2021 06:23
Operator : SY/MD
Sample : M4545-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

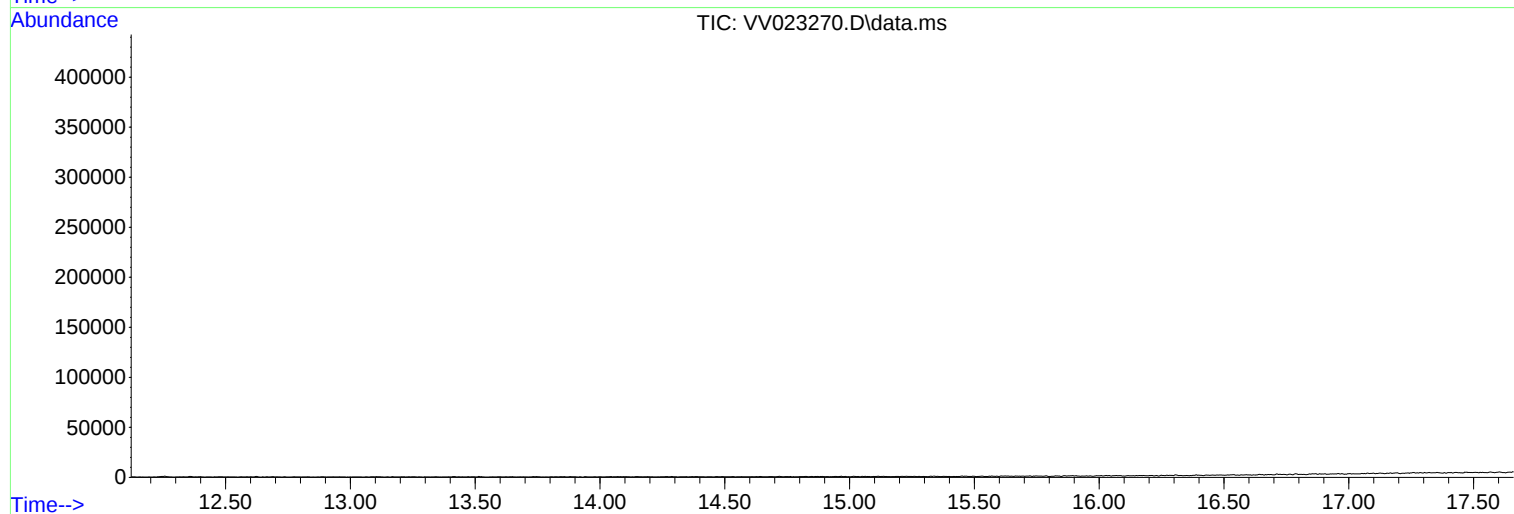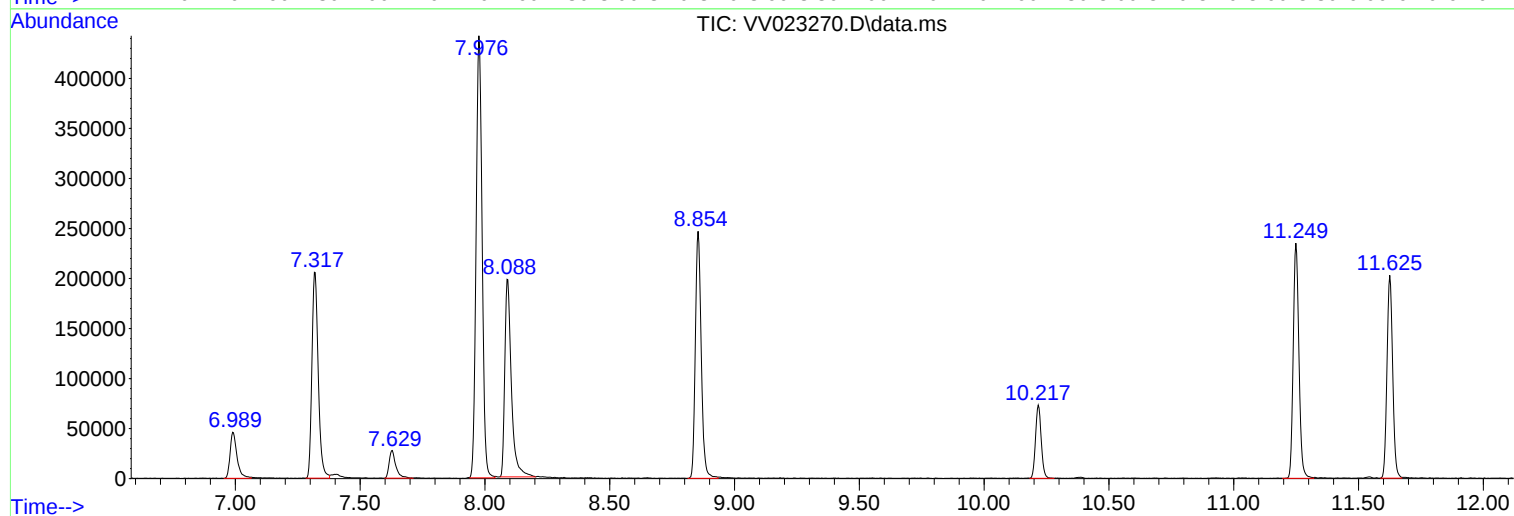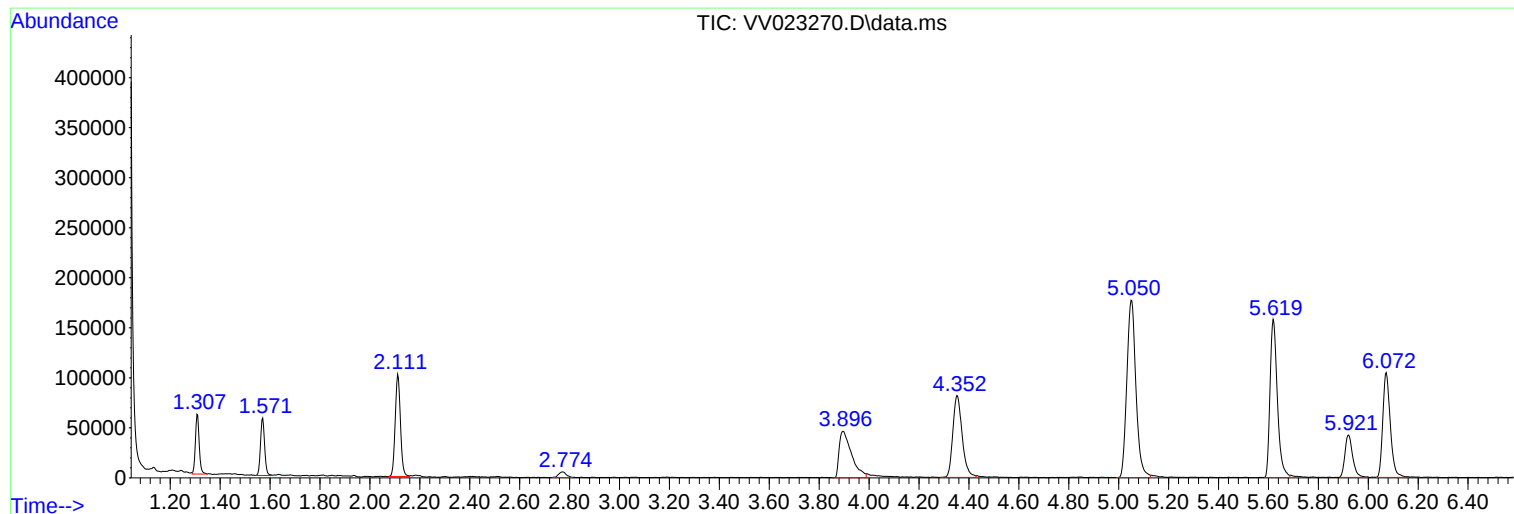

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023270.D
Acq On : 06 Nov 2021 06:23
Operator : SY/MD
Sample : M4545-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023270.D
Acq On : 06 Nov 2021 06:23
Operator : SY/MD
Sample : M4545-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4613

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
