


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110521\
Data File : VV023218.D
Acq On : 05 Nov 2021 09:27
Operator : SY/MD
Sample : BFB228
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB228

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 19 03:51:44 2021

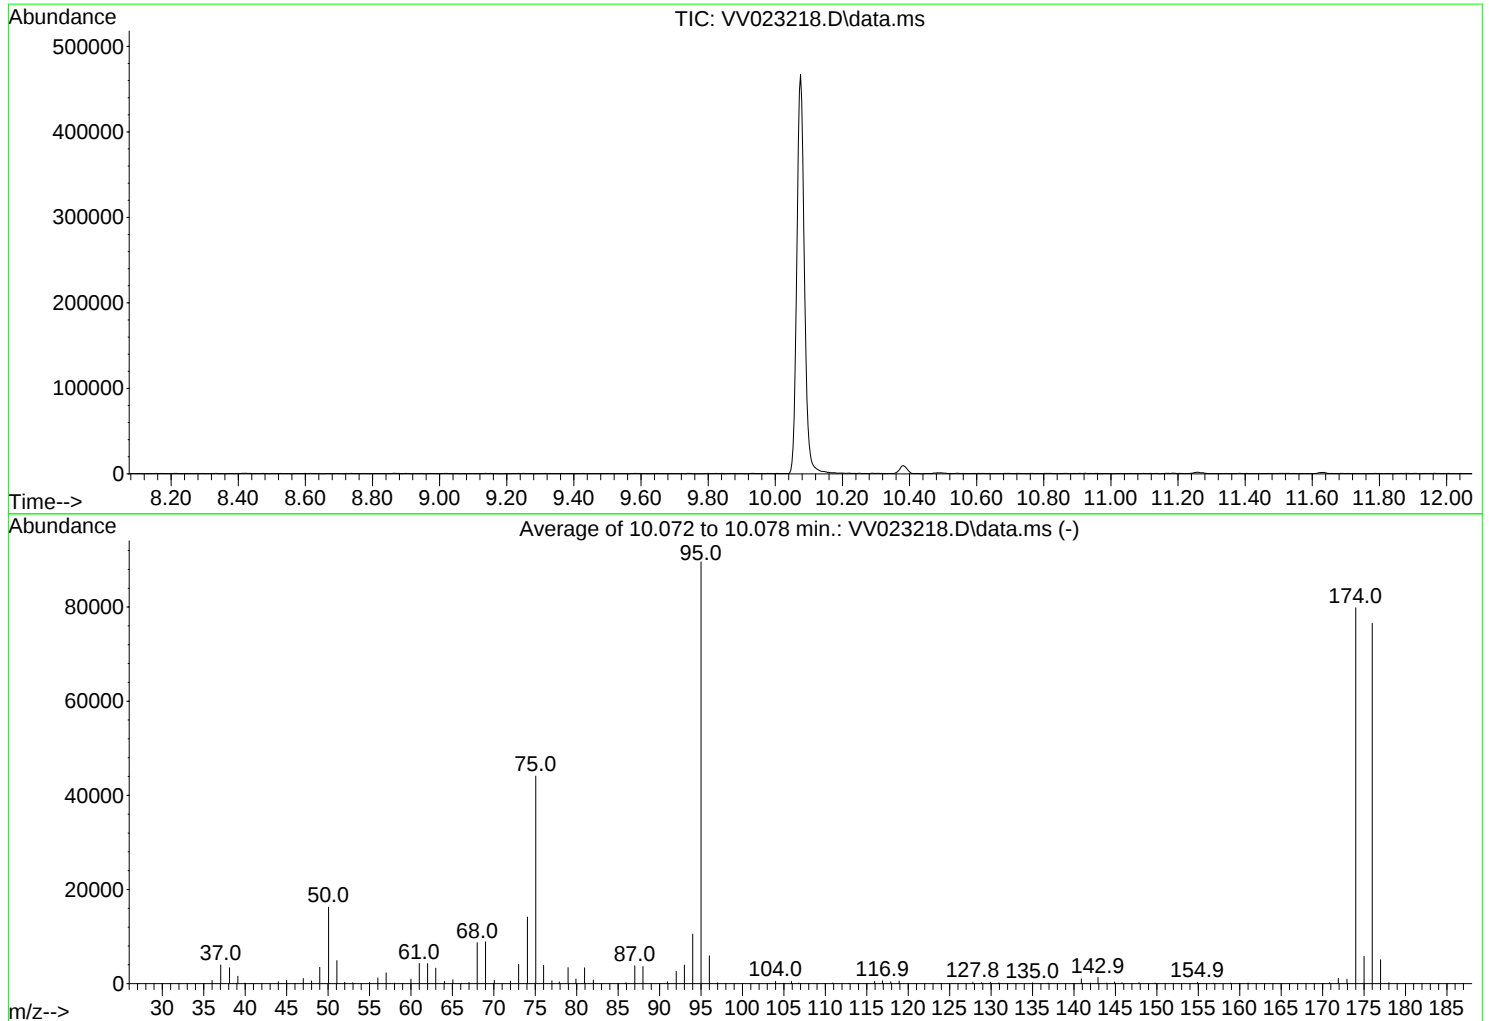

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	16247	PASS
75	95	30	80	49.2	44075	PASS
95	95	100	100	100.0	89603	PASS
96	95	5	9	6.6	5928	PASS
173	174	0.00	2	1.2	955	PASS
174	95	50	120	89.1	79832	PASS
175	174	5	9	7.3	5831	PASS
176	174	95	105	95.9	76547	PASS
177	176	5	10	6.6	5058	PASS

m/z	Abundance
39.90	137.0
43.10	111.0
44.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	664.0
37.00	4028.0
38.10	3455.0
39.10	1753.0
40.00	253.0
40.70	107.0
44.10	634.0
45.00	738.0
47.00	1158.0
48.00	569.0
49.00	3352.0
50.00	16512.0
51.00	4785.0
52.00	336.0
52.90	166.0
55.00	229.0
56.00	1201.0
57.00	2338.0
58.00	122.0
60.00	976.0
61.00	4186.0
62.00	4351.0
63.00	3288.0
64.00	510.0
65.00	832.0
66.00	116.0
67.00	229.0
68.00	8936.0
69.00	8793.0
70.00	788.0
72.00	471.0
73.00	3979.0
74.00	14475.0
75.00	44296.0
76.00	4115.0
77.00	543.0
77.90	335.0
78.90	3496.0
79.90	972.0
80.90	3472.0
82.00	786.0
86.00	212.0
87.00	3764.0
88.00	3784.0
90.90	408.0
92.00	2575.0
93.00	3925.0
94.00	10572.0
95.00	89960.0
96.00	5829.0
97.00	171.0
104.00	477.0
105.00	145.0
105.90	489.0
106.80	158.0
110.90	133.0
116.00	475.0
116.90	598.0
117.90	440.0
118.90	548.0
123.90	112.0
127.80	364.0
128.80	196.0
129.90	268.0
131.00	146.0
135.00	217.0
136.90	225.0
139.90	130.0
140.90	1026.0
142.10	152.0
142.90	1362.0
144.00	125.0
144.90	404.0
145.80	174.0
147.90	220.0
149.80	114.0
154.90	248.0
156.80	130.0
158.90	120.0
161.00	125.0
170.90	240.0
171.90	996.0
173.00	955.0
174.00	77888.0
175.00	5998.0
176.00	74288.0
177.00	4975.0
178.00	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	718.0
37.00	4139.0
38.10	3517.0
39.10	1624.0
40.00	282.0
44.10	626.0
45.00	758.0
46.00	114.0
47.00	1136.0
48.00	620.0
49.00	3645.0
50.10	16848.0
51.00	5059.0
52.00	337.0
53.00	183.0
55.00	196.0
56.00	1295.0
57.00	2335.0
58.00	138.0
60.00	1056.0
61.00	4483.0
62.00	4394.0
63.00	3356.0
64.00	477.0
65.10	833.0
66.10	123.0
67.00	271.0
68.00	9094.0
69.00	9196.0
70.10	756.0
72.00	567.0
73.00	4238.0
74.10	14579.0
75.10	45688.0
76.00	3987.0
77.00	616.0
77.90	406.0
78.90	3548.0
79.90	1033.0
81.00	3541.0
82.00	793.0
86.00	203.0
87.00	3971.0
88.00	3761.0
90.90	437.0
92.00	2700.0
93.00	4072.0
94.00	11010.0
95.00	92536.0
96.00	6083.0
97.00	168.0
104.00	513.0
105.00	126.0
105.90	479.0
106.80	160.0
110.80	125.0
112.80	111.0
115.90	482.0
116.90	635.0
117.90	428.0
118.90	593.0
123.80	107.0
127.80	333.0
128.80	229.0
129.90	325.0
130.90	214.0
135.00	210.0
136.90	212.0
140.90	1063.0
142.00	138.0
142.90	1285.0
144.00	136.0
144.90	375.0
145.80	212.0
147.80	241.0
149.80	168.0
154.90	299.0
156.80	115.0
158.90	128.0
161.00	150.0
170.10	108.0
170.80	193.0
171.90	1170.0
173.00	989.0
174.00	82536.0
175.00	5989.0
176.00	79488.0
177.00	5257.0
178.00	231.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
36.00	702.0
37.10	3725.0
38.10	3083.0
39.10	1373.0
40.00	299.0
44.00	558.0
45.00	686.0
46.00	134.0
47.00	1002.0
48.00	585.0
49.00	3422.0
50.10	15381.0
51.10	4831.0
52.00	267.0
53.00	184.0
55.00	196.0
56.00	1146.0
57.00	2241.0
58.10	146.0
60.00	978.0
61.00	4197.0
62.00	4048.0
63.00	3223.0
64.10	412.0
65.10	794.0
66.20	123.0
67.00	280.0
68.00	8048.0
69.00	8622.0
70.00	597.0
72.00	628.0
73.00	4025.0
74.10	13421.0
75.10	42240.0
76.00	3519.0
77.00	637.0
77.90	426.0
79.00	3214.0
79.90	990.0
81.00	3120.0
82.00	731.0
85.90	154.0
87.00	3659.0
88.00	3351.0
91.00	415.0
92.00	2561.0
93.00	3874.0
94.00	10080.0
95.00	86312.0
96.00	5872.0
97.00	221.0
104.00	445.0
105.90	413.0
106.80	127.0
110.80	123.0
112.80	109.0
115.90	438.0
116.90	630.0
117.90	389.0
118.90	563.0
127.80	293.0
128.90	201.0
129.90	334.0
130.90	230.0
135.00	178.0
137.10	162.0
140.90	954.0
141.90	143.0
142.90	1201.0
143.90	126.0
144.90	308.0
145.80	213.0
147.90	231.0
149.80	180.0
154.90	305.0
156.90	123.0
158.90	142.0
161.00	139.0
170.80	143.0
171.90	1195.0
172.90	921.0
174.00	79072.0
175.00	5505.0
176.00	75864.0
177.00	4942.0
178.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228