

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
 Data File : VV039337.D
 Acq On : 05 Nov 2025 15:50
 Operator : SY/MD
 Sample : Q3552-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 TB

Quant Time: Nov 06 00:16:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:01:26 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	4.596	168	856878	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	5.529	114	1636404	50.000	ug/l	0.00
63) Chlorobenzene-d5	8.773	117	1498704	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.172	152	661803	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	4.934	65	703372	57.768	ug/l	0.00
Spiked Amount	50.000	Range	81 - 118	Recovery	=	115.540%
35) Dibromofluoromethane	4.497	113	623292	48.341	ug/l	0.00
Spiked Amount	50.000	Range	80 - 119	Recovery	=	96.680%
50) Toluene-d8	7.233	98	2056521	46.884	ug/l	0.00
Spiked Amount	50.000	Range	89 - 112	Recovery	=	93.760%
62) 4-Bromofluorobenzene	9.998	95	679949	43.526	ug/l	0.00
Spiked Amount	50.000	Range	85 - 114	Recovery	=	87.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110525\
Data File : VV039337.D
Acq On : 05 Nov 2025 15:50
Operator : SY/MD
Sample : Q3552-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
TB

Quant Time: Nov 06 00:16:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V100725W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:01:26 2025
Response via : Initial Calibration

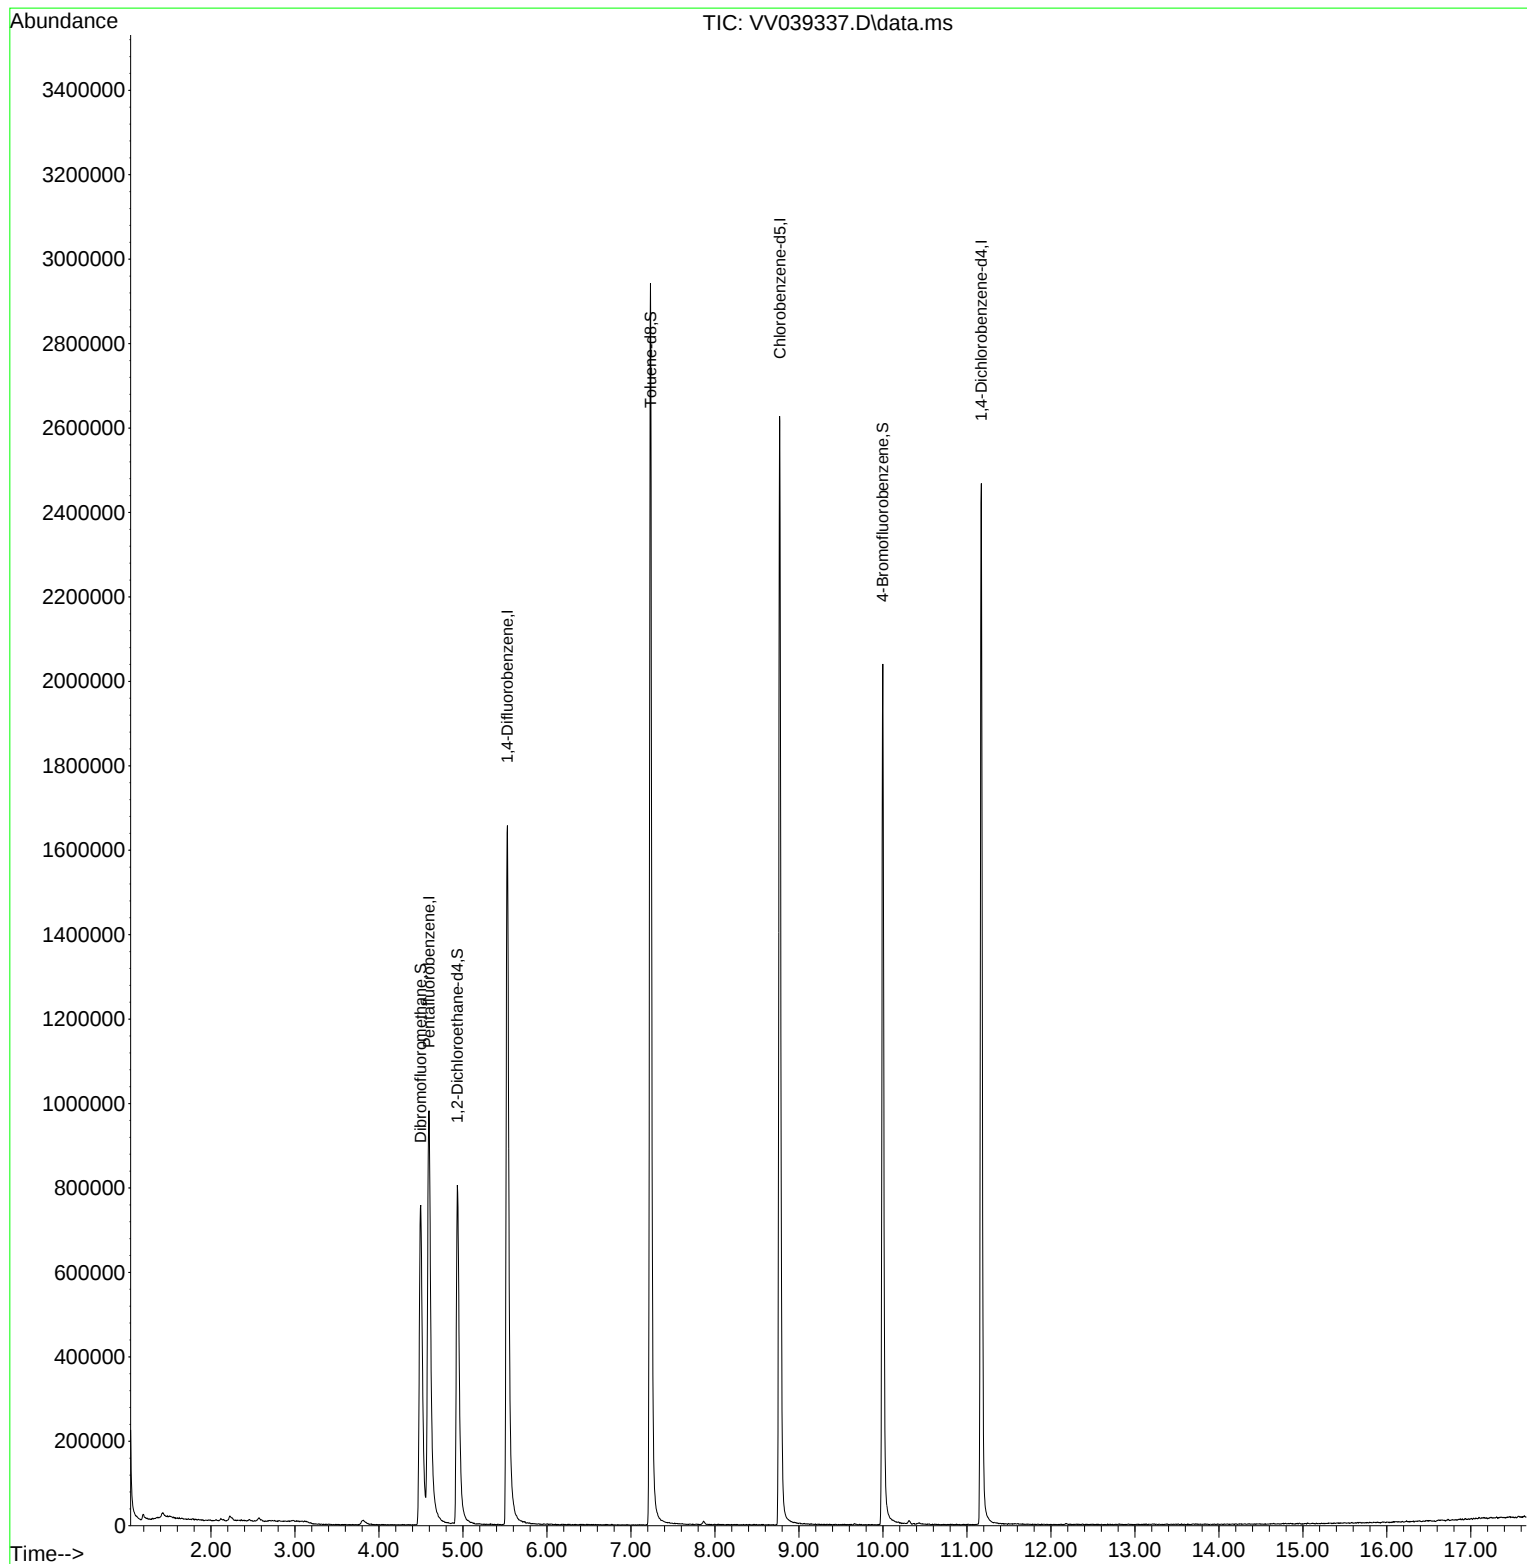

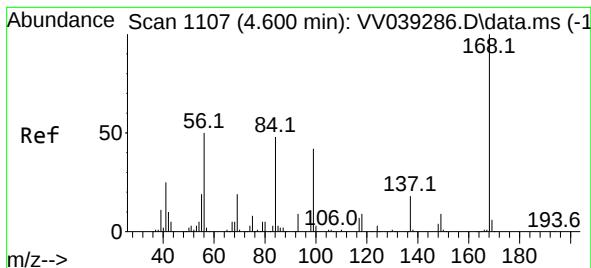

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.596 min Scan# 1106

Delta R.T. -0.004 min

Lab File: VV039337.D

Acq: 05 Nov 2025 15:50

Instrument :

MSVOA_V

ClientSampleId :





TB

Tgt Ion:168 Resp: 856878

Ion Ratio Lower Upper

168 100

99 59.8 46.6 70.0

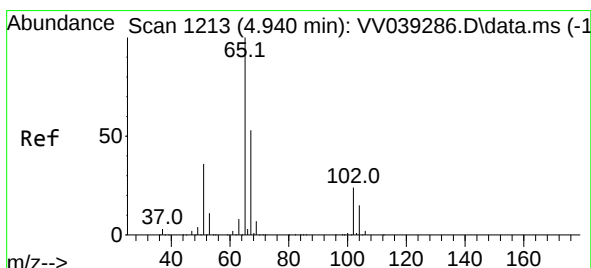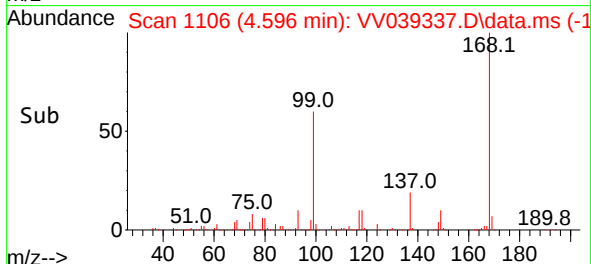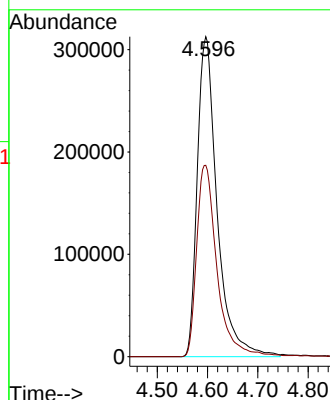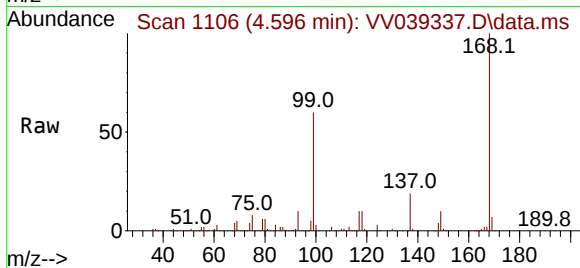

#33

1,2-Dichloroethane-d4

Concen: 57.768 ug/l

RT: 4.934 min Scan# 1211

Delta R.T. -0.006 min

Lab File: VV039337.D




Acq: 05 Nov 2025 15:50


Tgt Ion: 65 Resp: 703372

Ion Ratio Lower Upper

65 100

67 52.9 0.0 108.4


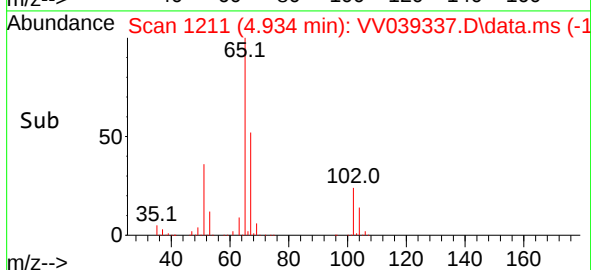
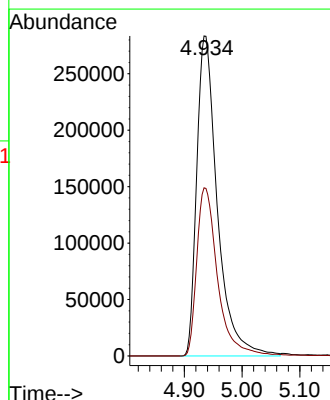
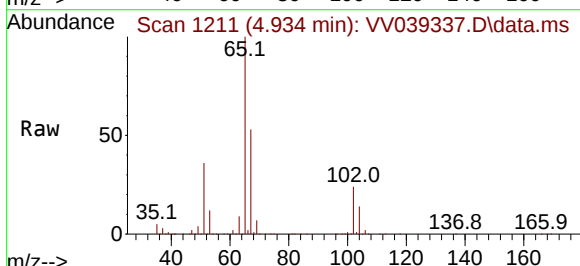


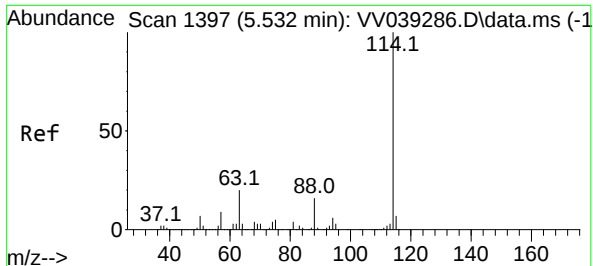

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 5.529 min Scan# 11
Delta R.T. -0.003 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50




Instrument :
MSVOA_V
ClientSampleId :
TB


Tgt Ion:114 Resp: 1636404
Ion Ratio Lower Upper
114 100
63 19.6 0.0 39.6
88 15.6 0.0 31.6

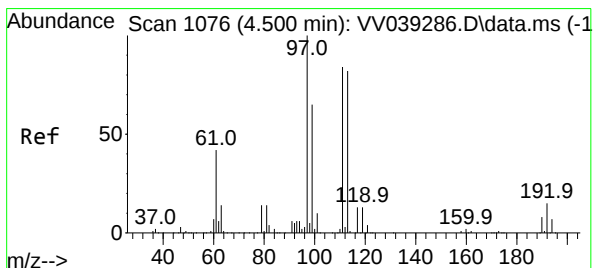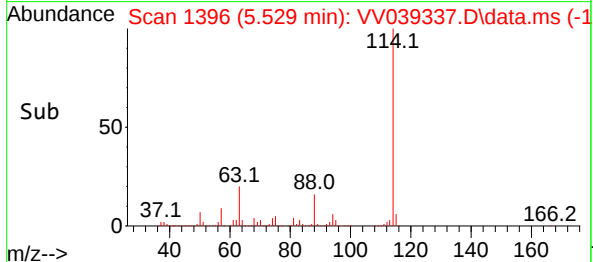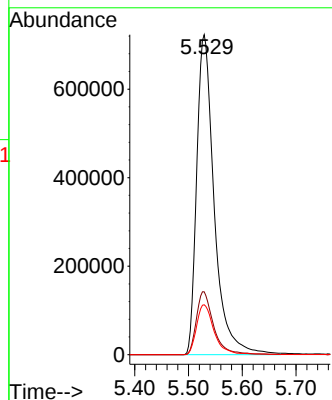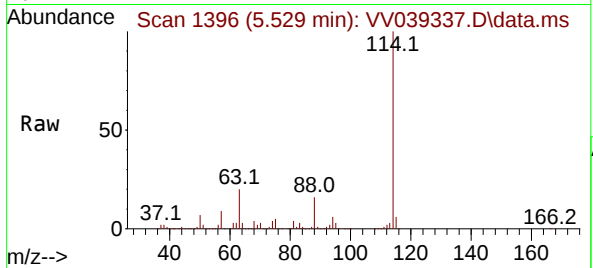

#35
Dibromofluoromethane
Concen: 48.341 ug/l
RT: 4.497 min Scan# 1075
Delta R.T. -0.003 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50

Tgt Ion:113 Resp: 623292
Ion Ratio Lower Upper
113 100
111 105.5 82.0 123.0
192 18.2 14.3 21.5


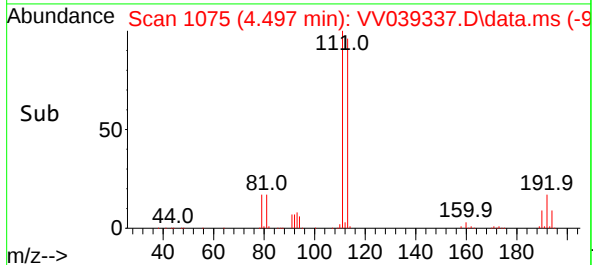
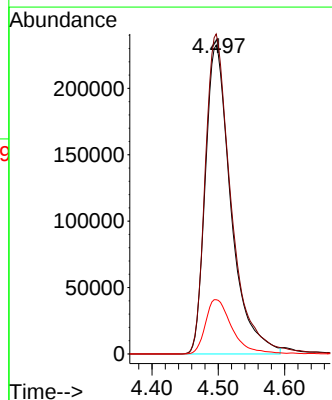
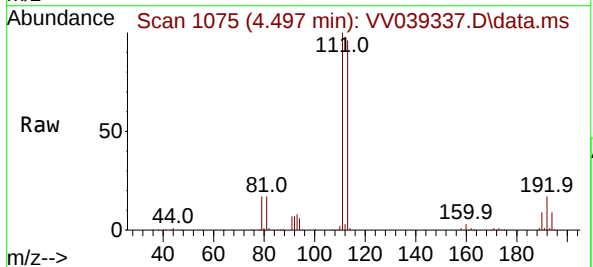


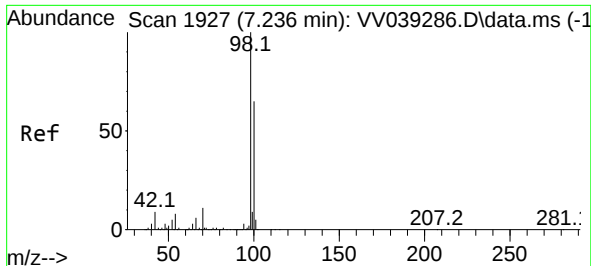

#50
Toluene-d8
Concen: 46.884 ug/l
RT: 7.233 min Scan# 1926
Delta R.T. -0.003 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50




Instrument :
MSVOA_V
ClientSampleId :
TB


Tgt Ion: 98 Resp: 2056521
Ion Ratio Lower Upper
98 100
100 64.6 52.8 79.2

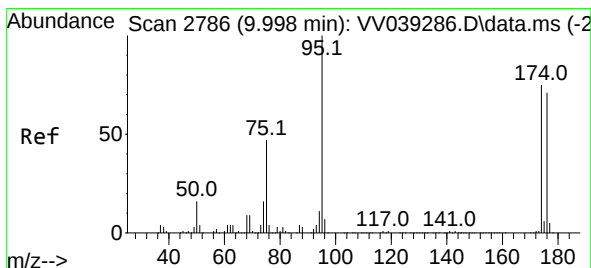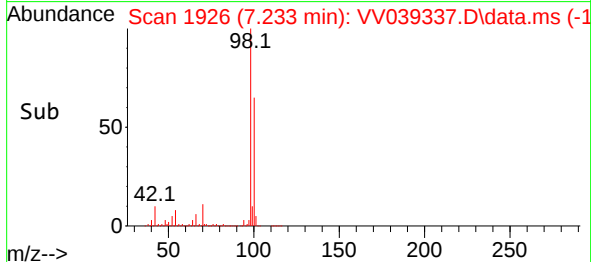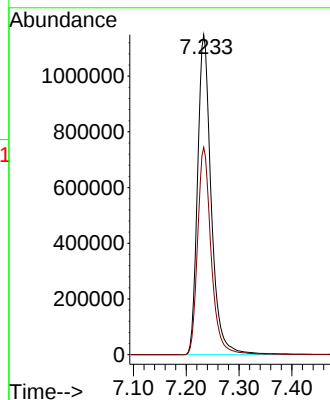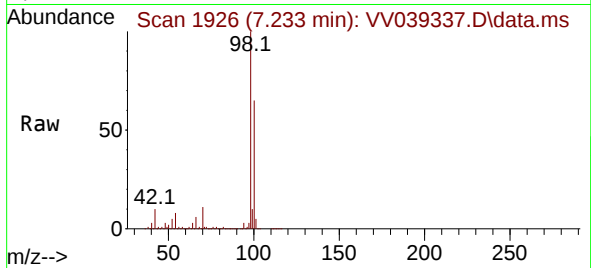

#62
4-Bromofluorobenzene
Concen: 43.526 ug/l
RT: 9.998 min Scan# 2786
Delta R.T. 0.000 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50

Tgt Ion: 95 Resp: 679949
Ion Ratio Lower Upper
95 100
174 79.8 0.0 153.6
176 74.6 0.0 146.0


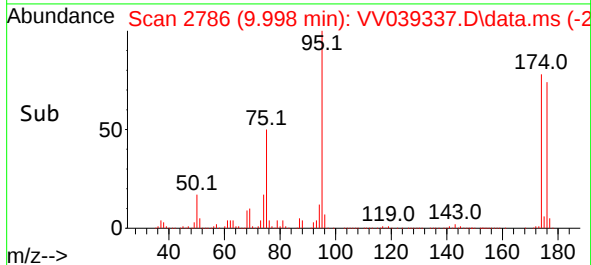
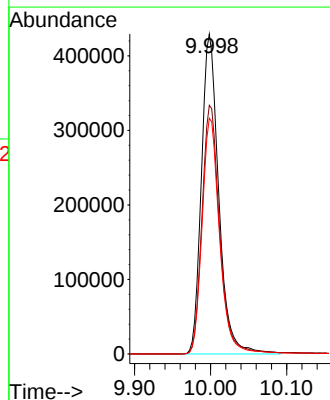
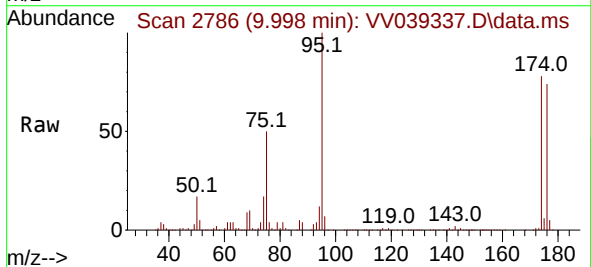


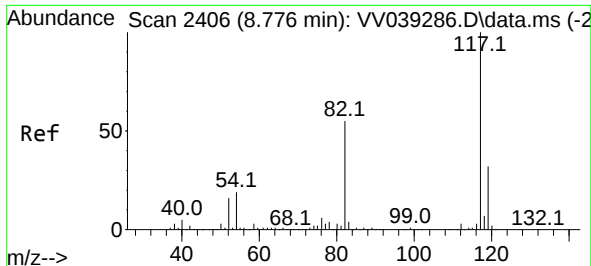

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 8.773 min Scan# 2405
Delta R.T. -0.003 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50

Instrument :
MSVOA_V
ClientSampleId :
TB

Tgt Ion:117 Resp: 1498704
Ion Ratio Lower Upper
117 100
82 54.6 43.8 65.8
119 32.2 25.8 38.6

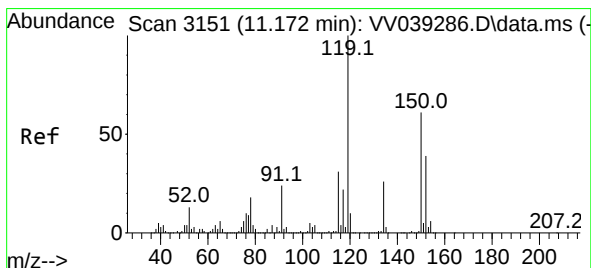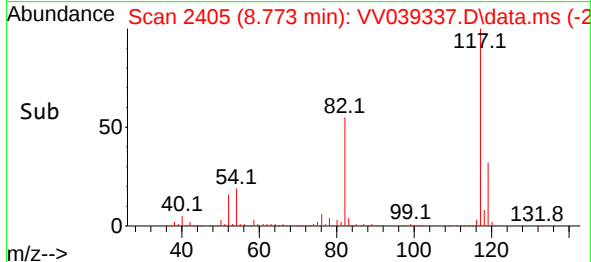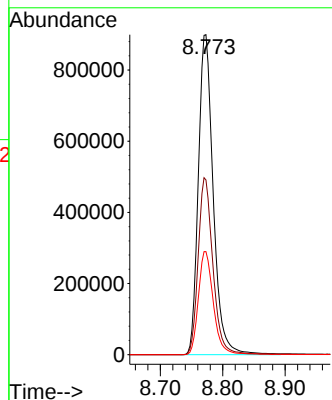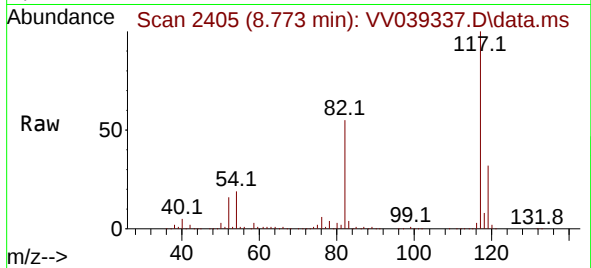

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.172 min Scan# 3151
Delta R.T. 0.000 min
Lab File: VV039337.D
Acq: 05 Nov 2025 15:50

Tgt Ion:152 Resp: 661803
Ion Ratio Lower Upper
152 100
115 61.3 42.3 126.8
150 158.6 0.0 348.0

