


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110620\
 Data File : VV019256.D
 Acq On : 04 Nov 2020 19:11
 Operator : SY/MD
 Sample : BFB61
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB304

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM110320WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 05 04:58:48 2020

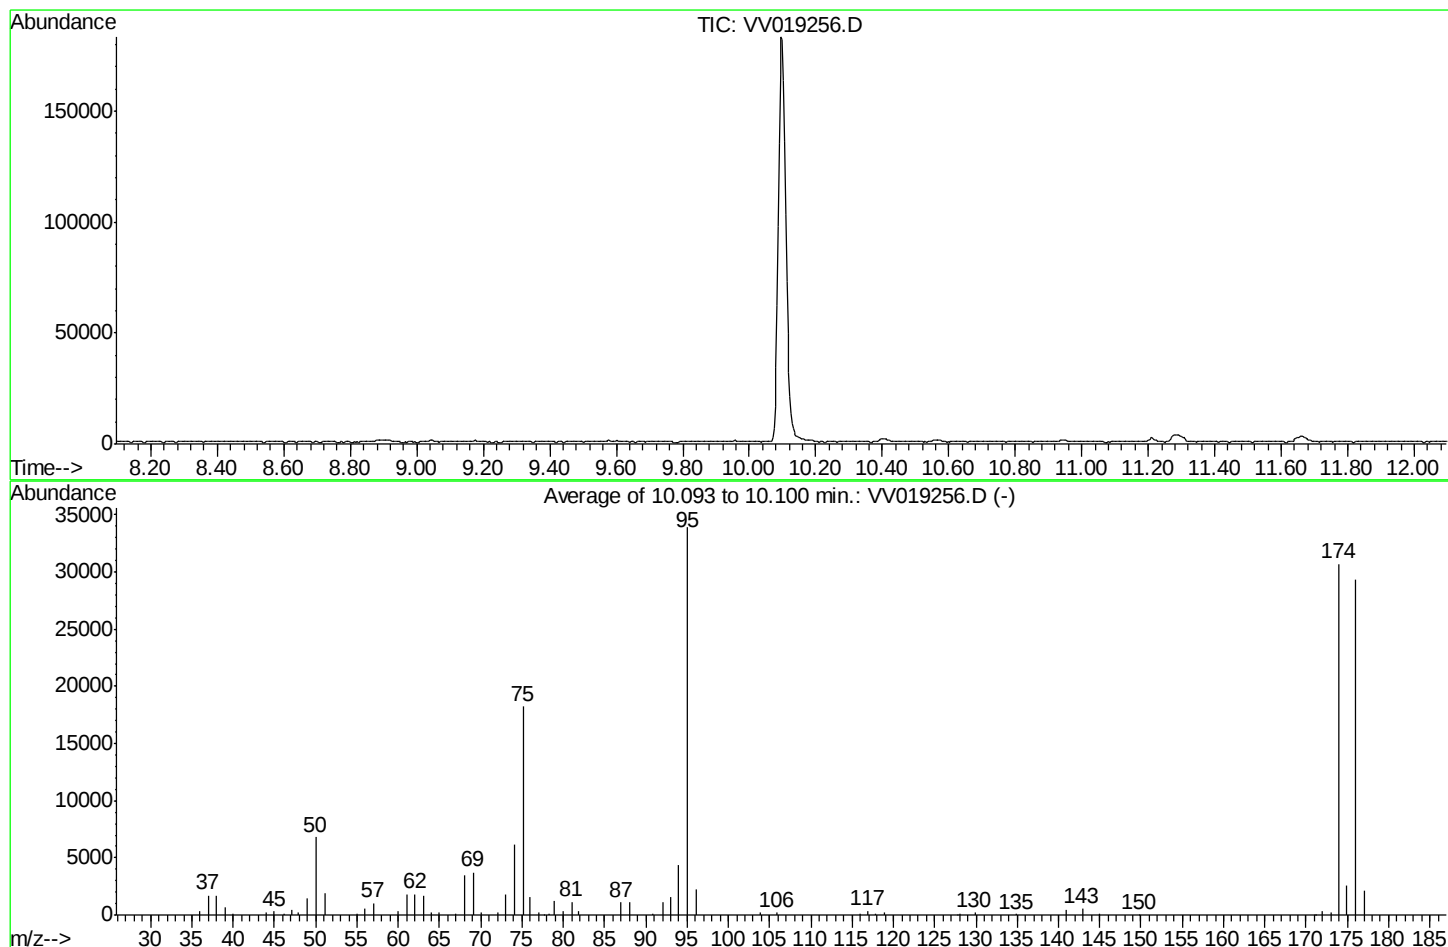

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6820	PASS
75	95	30	80	53.7	18210	PASS
95	95	100	100	100.0	33914	PASS
96	95	5	9	6.5	2198	PASS
173	174	0.00	2	0.6	193	PASS
174	95	50	120	90.6	30733	PASS
175	174	5	9	8.3	2550	PASS
176	174	95	101	95.4	29330	PASS
177	176	5	9	7.2	2099	PASS

Scan 2790 (10.061 min): VV019256.D
BFB61

m/z	Abundance
40.00	117.0
44.00	814.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
35.90	342.0
37.00	1725.0
38.00	1691.0
39.00	603.0
40.00	169.0
44.00	1156.0
45.00	322.0
46.20	140.0
47.10	361.0
47.90	195.0
49.00	1590.0
50.00	6910.0
51.00	1883.0
56.00	515.0
57.00	1017.0
60.00	334.0
61.00	1755.0
62.00	1861.0
63.00	1731.0
64.00	225.0
65.00	221.0
66.90	111.0
68.00	3703.0
69.10	3780.0
70.00	244.0
72.00	234.0
73.00	1847.0
74.10	6249.0
75.10	18456.0
76.00	1619.0
77.00	231.0
78.90	1297.0
79.90	407.0
81.00	1242.0
81.90	276.0
87.00	1210.0
88.00	1169.0
90.80	206.0
92.00	1199.0
93.00	1531.0
94.00	4509.0
95.00	34000.0
96.10	2173.0
103.80	167.0
105.90	227.0
115.90	149.0
116.90	367.0
117.80	163.0
118.90	242.0
128.00	196.0
129.90	190.0
134.90	108.0
140.90	452.0
142.90	537.0
145.00	140.0
149.80	109.0
171.90	367.0
173.10	579.0
174.00	32000.0
174.90	2621.0
176.00	31152.0
177.00	2130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
35.90	328.0
37.00	1753.0
38.00	1713.0
39.00	633.0
40.00	194.0
44.00	1050.0
45.00	286.0
46.10	141.0
47.10	454.0
47.90	250.0
49.00	1499.0
50.00	7005.0
51.10	1978.0
55.00	122.0
55.90	570.0
57.00	1064.0
60.00	397.0
61.00	1795.0
62.00	1915.0
63.00	1765.0
64.00	223.0
65.00	259.0
66.90	120.0
68.00	3584.0
69.10	3831.0
70.00	229.0
72.00	250.0
73.00	1860.0
74.10	6403.0
75.10	18816.0
76.00	1647.0
77.00	299.0
77.70	107.0
78.20	145.0
79.00	1305.0
80.00	355.0
81.00	1208.0
81.90	280.0
87.00	1141.0
88.00	1119.0
90.80	170.0
92.00	1161.0
93.00	1625.0
94.00	4519.0
95.00	35104.0
96.00	2309.0
103.80	195.0
105.90	229.0
115.90	124.0
116.90	355.0
117.90	166.0
118.90	285.0
128.00	152.0
129.90	195.0
134.90	116.0
140.90	414.0
142.90	530.0
144.90	158.0
171.20	107.0
171.90	366.0
174.00	31880.0
175.00	2661.0
176.00	30376.0
177.00	2193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304

m/z	Abundance
35.90	292.0
37.00	1637.0
38.00	1587.0
39.00	685.0
40.00	211.0
44.00	968.0
45.00	251.0
46.00	126.0
47.10	393.0
47.90	276.0
49.00	1284.0
50.00	6545.0
51.10	1902.0
55.10	125.0
55.90	550.0
57.00	982.0
60.00	407.0
61.00	1705.0
62.00	1724.0
63.00	1554.0
64.00	227.0
65.00	268.0
66.90	112.0
68.00	3251.0
69.00	3616.0
70.00	250.0
72.00	235.0
73.00	1674.0
74.00	5742.0
75.10	17360.0
76.00	1590.0
77.00	297.0
78.20	169.0
79.00	1154.0
80.00	308.0
81.00	1041.0
81.90	297.0
87.00	973.0
88.00	970.0
90.80	139.0
92.00	1084.0
93.00	1581.0
94.00	4205.0
95.10	32640.0
96.00	2112.0
103.80	196.0
105.90	213.0
115.90	109.0
116.90	307.0
117.90	171.0
118.90	276.0
127.80	127.0
129.90	155.0
140.90	342.0
142.90	511.0
144.90	169.0
171.00	149.0
171.90	353.0
174.00	28320.0
175.00	2370.0
176.00	26464.0
177.00	1975.0

Instrument :
MSVOA_V
ClientSampleId :
BFB304