

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110623\
 Data File : VW032852.D
 Acq On : 06 Nov 2023 14:29
 Operator : SY/MD
 Sample : 05203-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 07 01:36:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 07 01:35:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	349760	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	362526	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	166261	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	104430	31.392	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	62.780%
7) Chloroethane-d5	1.510	69	113278	40.714	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.420%
11) 1,1-Dichloroethene-d2	2.053	65	53417	38.875	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.760%
21) 2-Butanone-d5	3.786	46	122064	84.593	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.590%
24) Chloroform-d	4.249	84	229796	43.277	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.560%
26) 1,2-Dichloroethane-d4	4.940	65	155994	47.268	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.540%
32) Benzene-d6	4.960	84	444588	47.697	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	5.989	67	138466	48.897	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.800%
41) Toluene-d8	7.243	98	392165	42.728	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.460%
43) trans-1,3-Dichloroprop...	7.555	79	65536	44.436	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.880%
47) 2-Hexanone-d5	8.027	63	98854	95.621	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.620%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	203180	47.282	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.560%
66) 1,2-Dichlorobenzene-d4	11.564	152	173521	54.158	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.320%
Target Compounds						
44) trans-1,3-Dichloropropene	7.555	75	3645	0.927	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032852.D
Acq On : 06 Nov 2023 14:29
Operator : SY/MD
Sample : 05203-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 07 01:36:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 07 01:35:20 2023
Response via : Initial Calibration

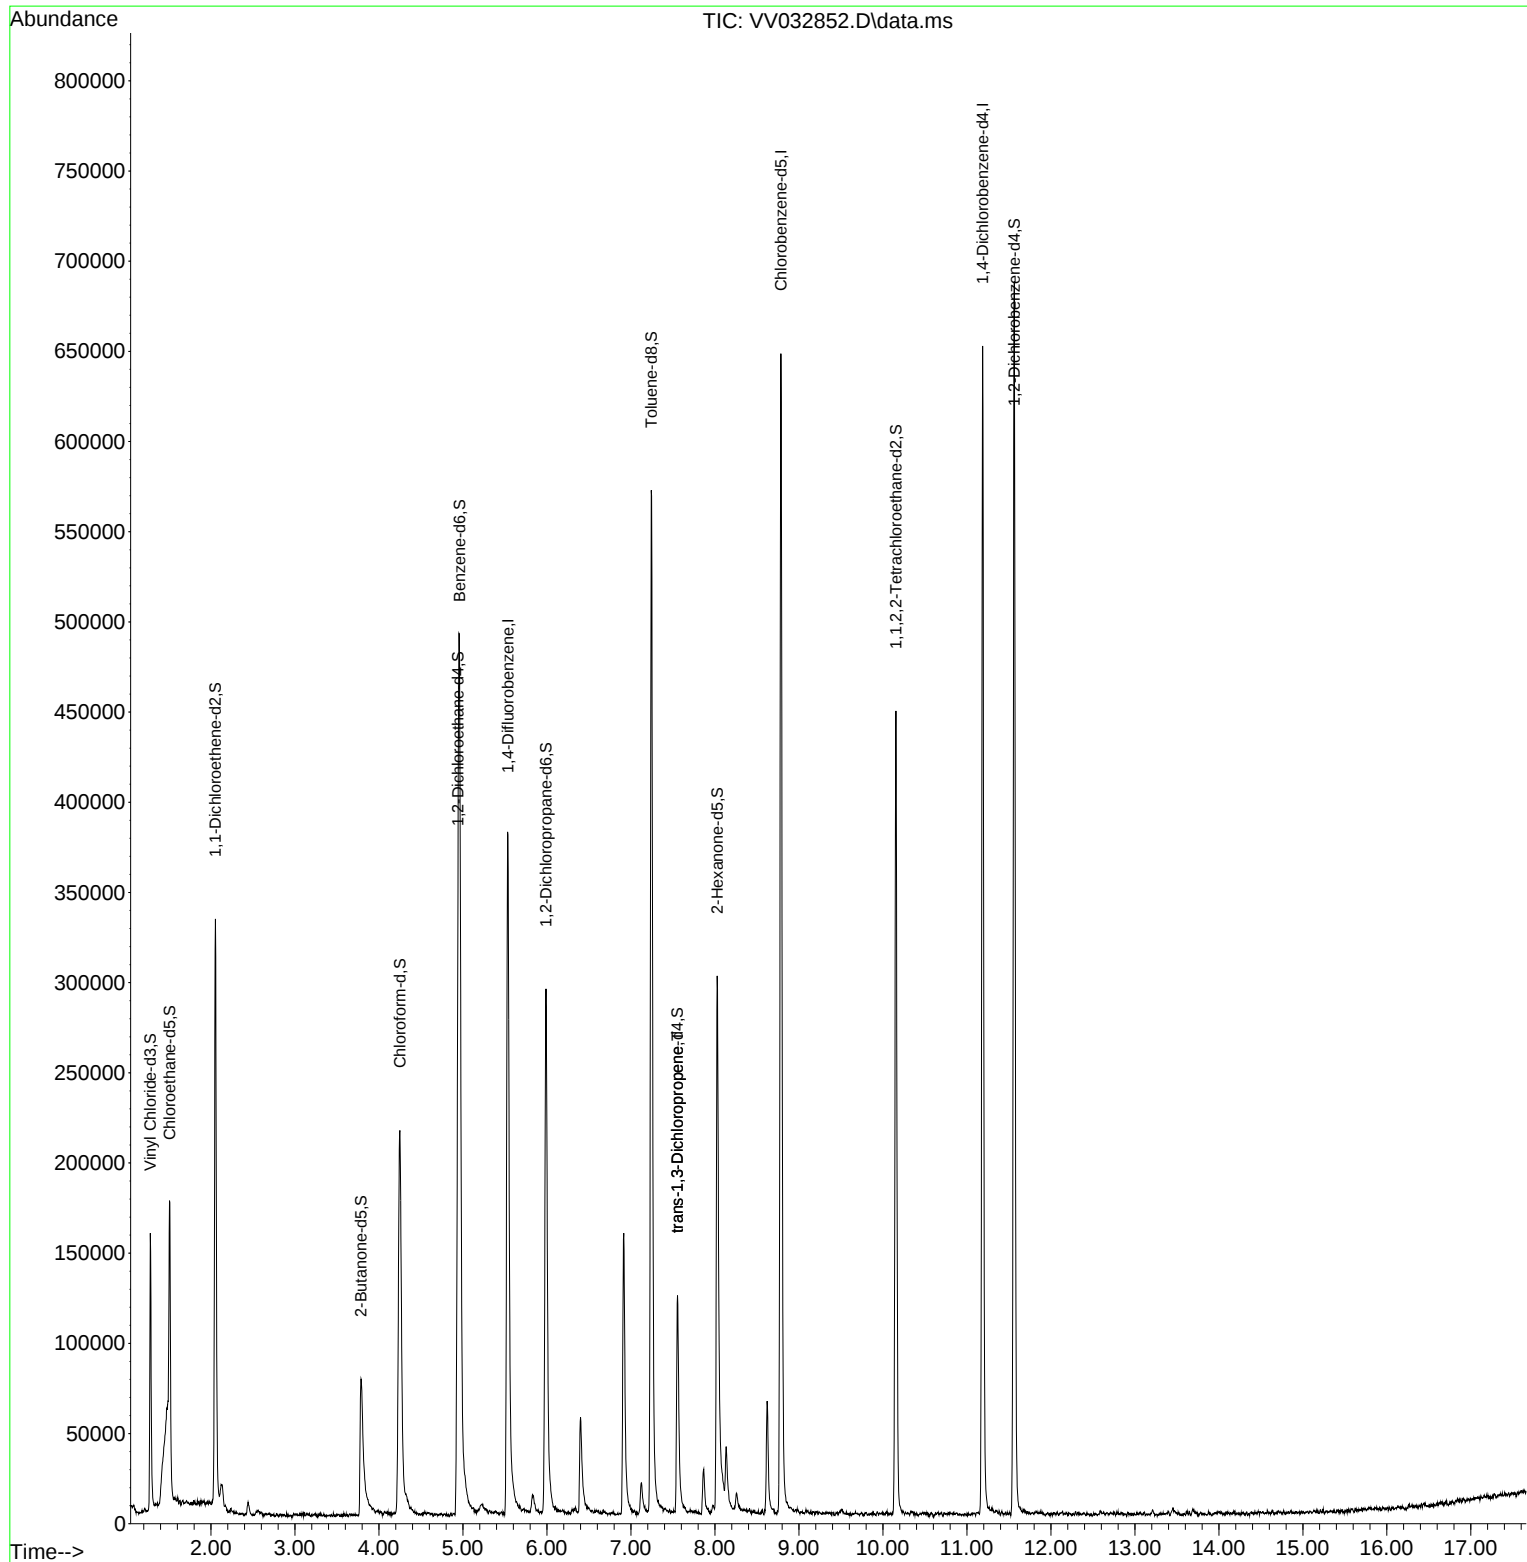

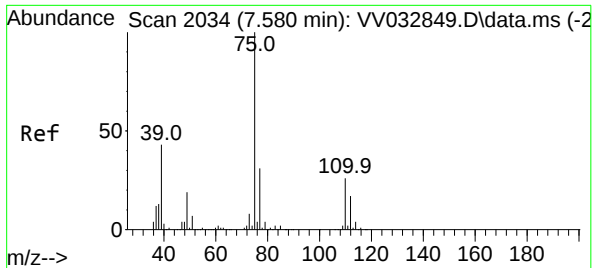

#44
 trans-1,3-Dichloropropene
 Concen: 0.927 ug/L
 RT: 7.555 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV032852.D
 Acq: 06 Nov 2023 14:29

Instrument :
 MSVOA_V
 ClientSampleId :

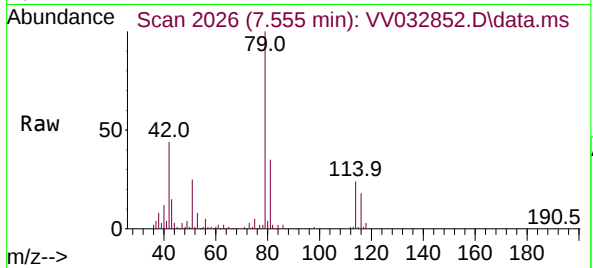

Tgt Ion: 75 Resp: 3645
 Ion Ratio Lower Upper
 75 100
 77 39.9 22.0 40.8

