

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032853.D
 Acq On : 06 Nov 2023 15:11
 Operator : SY/MD
 Sample : 05203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 07 01:36:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 07 01:35:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	337990	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	375248	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	170634	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	117682	36.607	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	73.220%	
7) Chloroethane-d5	1.532	69	109376	40.681	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	81.360%	
11) 1,1-Dichloroethene-d2	2.059	65	52368	39.439	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.880%	
21) 2-Butanone-d5	3.783	46	121184	86.908	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	86.910%	
24) Chloroform-d	4.249	84	233268	45.460	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.920%	
26) 1,2-Dichloroethane-d4	4.940	65	146426	45.914	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.820%	
32) Benzene-d6	4.960	84	428136	44.375	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.740%	
36) 1,2-Dichloropropane-d6	5.989	67	138443	47.231	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.460%	
41) Toluene-d8	7.243	98	404279	42.555	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.100%	
43) trans-1,3-Dichloroprop...	7.554	79	68402	44.807	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.620%	
47) 2-Hexanone-d5	8.027	63	87087	81.383	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	81.380%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	202316	45.485	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.960%	
66) 1,2-Dichlorobenzene-d4	11.564	152	171372	52.117	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.240%	
Target Compounds						
39) cis-1,3-Dichloropropene	6.918	75	4763	1.202	ug/L	Qvalue # 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032853.D
Acq On : 06 Nov 2023 15:11
Operator : SY/MD
Sample : 05203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 07 01:36:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 07 01:35:20 2023
Response via : Initial Calibration

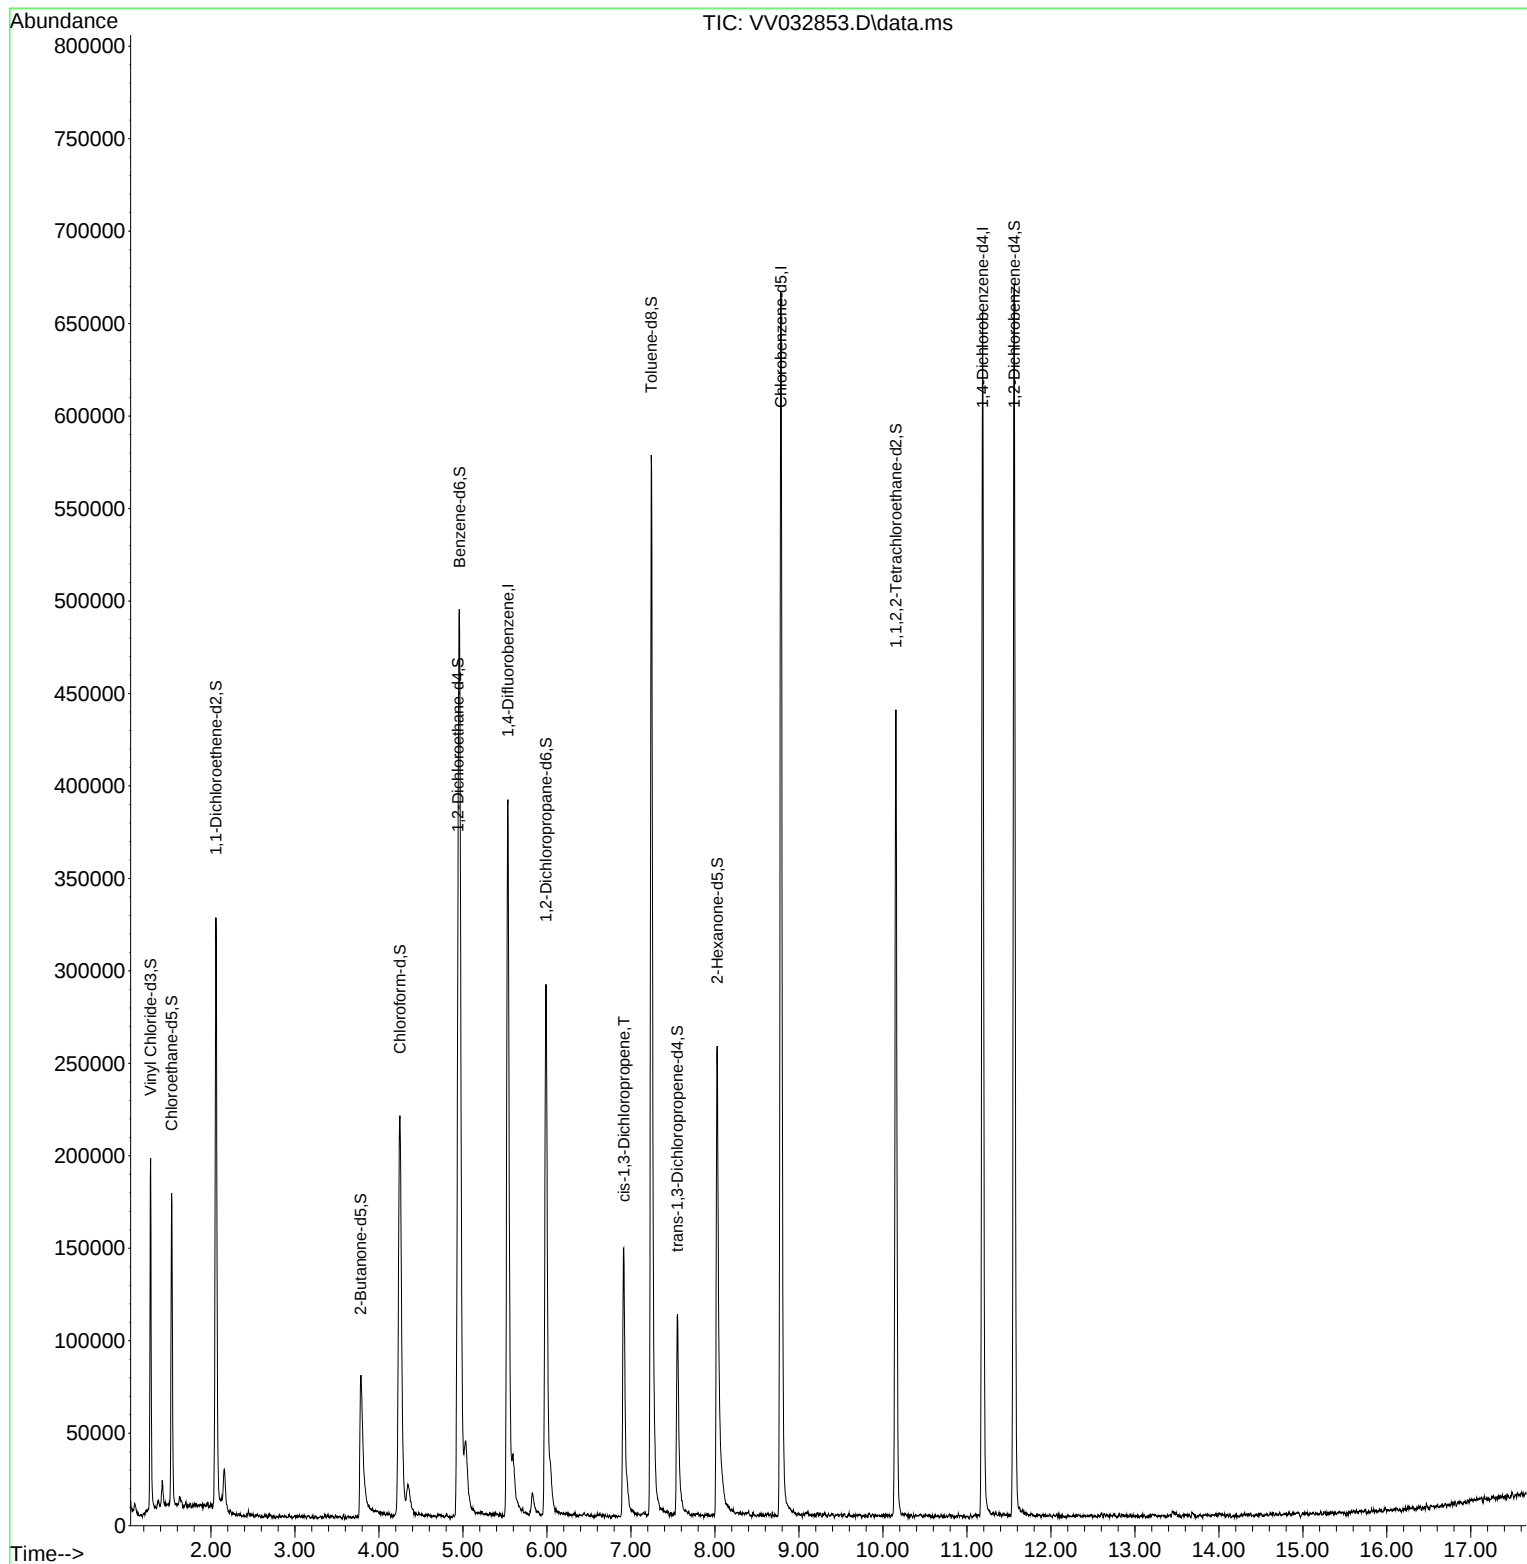

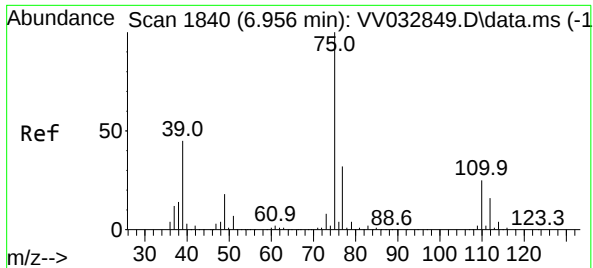

#39
 cis-1,3-Dichloropropene
 Concen: 1.202 ug/L
 RT: 6.918 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV032853.D
 Acq: 06 Nov 2023 15:11

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75	Resp: 4763
Ion Ratio	Lower Upper
75	100
77	44.1 23.0 42.8#

