

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032850.D
 Acq On : 06 Nov 2023 13:23
 Operator : SY/MD
 Sample : VV1106WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	181296	192964	14.71%	1.801%
2	1.532	147	153	163	rVB	165929	190836	14.55%	1.781%
3	2.063	309	318	331	rVB	316838	452599	34.50%	4.224%
4	2.343	403	405	408	rBV4	2139	1010	0.08%	0.009%
5	2.642	496	498	500	rBV3	1172	543	0.04%	0.005%
6	2.658	500	503	504	rBV2	1538	713	0.05%	0.007%
7	2.728	523	525	527	rBV3	1925	767	0.06%	0.007%
8	2.809	549	550	551	rBV	1376	438	0.03%	0.004%
9	2.873	568	570	573	rBV3	1091	695	0.05%	0.006%
10	2.915	581	583	585	rBV3	1879	1138	0.09%	0.011%
11	3.063	626	629	630	rBV2	1538	914	0.07%	0.009%
12	3.073	630	632	635	rVV3	1421	902	0.07%	0.008%
13	3.127	646	649	650	rBV3	1465	703	0.05%	0.007%
14	3.188	667	668	669	rBV	707	182	0.01%	0.002%
15	3.333	711	713	716	rBV4	979	609	0.05%	0.006%
16	3.359	719	721	726	rVB6	1256	920	0.07%	0.009%
17	3.381	726	728	729	rBV2	864	412	0.03%	0.004%
18	3.510	766	768	770	rBV3	1511	685	0.05%	0.006%
19	3.523	770	772	774	rVB2	1732	572	0.04%	0.005%
20	3.532	774	775	776	rBV	665	197	0.02%	0.002%
21	3.648	808	811	813	rBV4	784	397	0.03%	0.004%
22	3.661	813	815	817	rVV3	1171	382	0.03%	0.004%
23	3.728	831	836	838	rBV6	2355	1922	0.15%	0.018%
24	3.754	843	844	845	rBV	980	276	0.02%	0.003%
25	3.786	845	854	878	rBV	83105	227850	17.37%	2.126%
26	4.253	980	999	1019	rBV	223262	585860	44.66%	5.467%
27	4.503	1075	1077	1078	rBV2	1575	634	0.05%	0.006%
28	4.683	1130	1133	1139	rBV8	2072	2159	0.16%	0.020%
29	4.818	1173	1175	1177	rBV3	1343	752	0.06%	0.007%
30	4.860	1186	1188	1189	rBV2	1070	358	0.03%	0.003%
31	4.883	1192	1195	1197	rVV4	2252	1221	0.09%	0.011%
32	4.960	1203	1219	1235	rBV2	494968	1311848	100.00%	12.242%
33	5.535	1387	1398	1415	rBV	394023	817625	62.33%	7.630%
34	5.989	1528	1539	1574	rBV	290798	651380	49.65%	6.079%
35	6.249	1617	1620	1622	rVB3	1897	916	0.07%	0.009%
36	6.265	1622	1625	1628	rBV5	1665	1145	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032850.D
 Acq On : 06 Nov 2023 13:23
 Operator : SY/MD
 Sample : VV1106WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.799	1789	1791	1792	rBV2	995	483	0.04%	0.005%
38	6.915	1813	1827	1854	rBV	147148	308318	23.50%	2.877%
39	7.246	1919	1930	1963	rBV	579893	1091194	83.18%	10.183%
40	7.555	2018	2026	2046	rBV	109164	200569	15.29%	1.872%
41	7.770	2091	2093	2096	rBV4	1182	506	0.04%	0.005%
42	7.844	2112	2116	2119	rBV6	2185	1724	0.13%	0.016%
43	7.883	2126	2128	2131	rBV4	1291	564	0.04%	0.005%
44	7.963	2151	2153	2155	rBV3	1493	769	0.06%	0.007%
45	8.027	2164	2173	2207	rBV	281021	607624	46.32%	5.670%
46	8.690	2375	2379	2382	rBV5	1622	1532	0.12%	0.014%
47	8.786	2398	2409	2429	rBV	671175	1137994	86.75%	10.620%
48	9.217	2541	2543	2545	rBV3	1190	397	0.03%	0.004%
49	9.310	2568	2572	2574	rBV4	2019	1351	0.10%	0.013%
50	9.397	2596	2599	2603	rBV6	3022	2213	0.17%	0.021%
51	9.982	2779	2781	2783	rVB3	1256	407	0.03%	0.004%
52	10.008	2786	2789	2791	rBV3	1852	1276	0.10%	0.012%
53	10.085	2810	2813	2816	rBV5	1637	1100	0.08%	0.010%
54	10.114	2820	2822	2823	rBV2	1360	440	0.03%	0.004%
55	10.156	2823	2835	2853	rVV	453391	719087	54.81%	6.710%
56	10.455	2923	2928	2932	rBV7	1940	2202	0.17%	0.021%
57	10.474	2932	2934	2936	rBV3	1378	730	0.06%	0.007%
58	10.551	2956	2958	2964	rVB7	2470	1912	0.15%	0.018%
59	10.667	2992	2994	2996	rBV3	1056	547	0.04%	0.005%
60	10.722	3009	3011	3012	rBV2	1182	530	0.04%	0.005%
61	10.783	3028	3030	3032	rBV3	1836	862	0.07%	0.008%
62	10.841	3046	3048	3049	rBV2	970	271	0.02%	0.003%
63	10.908	3067	3069	3070	rVB2	1313	366	0.03%	0.003%
64	11.188	3145	3156	3179	rBV	683758	1051457	80.15%	9.812%
65	11.564	3261	3273	3291	rBV	683610	1089572	83.06%	10.168%
66	11.738	3325	3327	3328	rBV2	1556	514	0.04%	0.005%
67	12.034	3417	3419	3421	rBV2	1924	875	0.07%	0.008%
68	12.046	3421	3423	3425	rVB3	1553	579	0.04%	0.005%
69	12.140	3450	3452	3455	rBV4	1947	1062	0.08%	0.010%
70	12.249	3484	3486	3490	rVB5	1248	896	0.07%	0.008%
71	12.516	3566	3569	3570	rBV2	1626	835	0.06%	0.008%
72	12.757	3641	3644	3646	rBV4	1664	944	0.07%	0.009%
73	12.844	3669	3671	3672	rBV2	698	272	0.02%	0.003%
74	12.879	3677	3682	3683	rBV4	1975	1778	0.14%	0.017%
75	13.210	3777	3785	3795	rBV4	4951	7867	0.60%	0.073%
76	13.281	3804	3807	3809	rBV3	1522	977	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032850.D
Acq On : 06 Nov 2023 13:23
Operator : SY/MD
Sample : VV1106WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	13.297	3809	3812	3815	rBV4	2306	1807	0.14%	0.017%
78	13.355	3828	3830	3833	rVB4	1025	469	0.04%	0.004%
79	13.371	3833	3835	3838	rBV3	1141	765	0.06%	0.007%
80	13.689	3927	3934	3942	rBV3	6353	8661	0.66%	0.081%
81	14.030	4037	4040	4042	rBV4	1765	1239	0.09%	0.012%
82	14.124	4067	4069	4070	rBV2	1782	722	0.06%	0.007%
83	14.159	4076	4080	4082	rBV5	1459	1116	0.09%	0.010%
84	14.249	4106	4108	4112	rVB5	1850	913	0.07%	0.009%
85	14.268	4112	4114	4118	rVB3	2279	1122	0.09%	0.010%
86	14.435	4164	4166	4167	rBV2	1199	659	0.05%	0.006%
87	14.471	4175	4177	4178	rBV2	1465	510	0.04%	0.005%
88	14.815	4278	4284	4285	rBV6	2748	2755	0.21%	0.026%




Sum of corrected areas: 10715858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032850.D
Acq On : 06 Nov 2023 13:23
Operator : SY/MD
Sample : VV1106WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

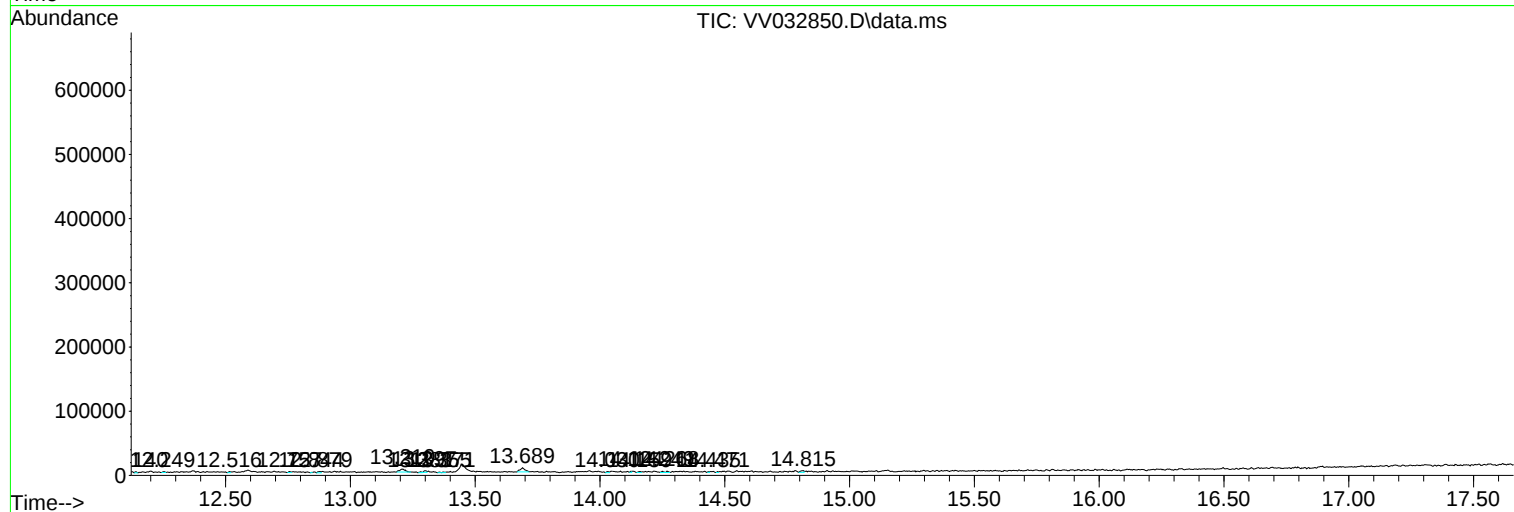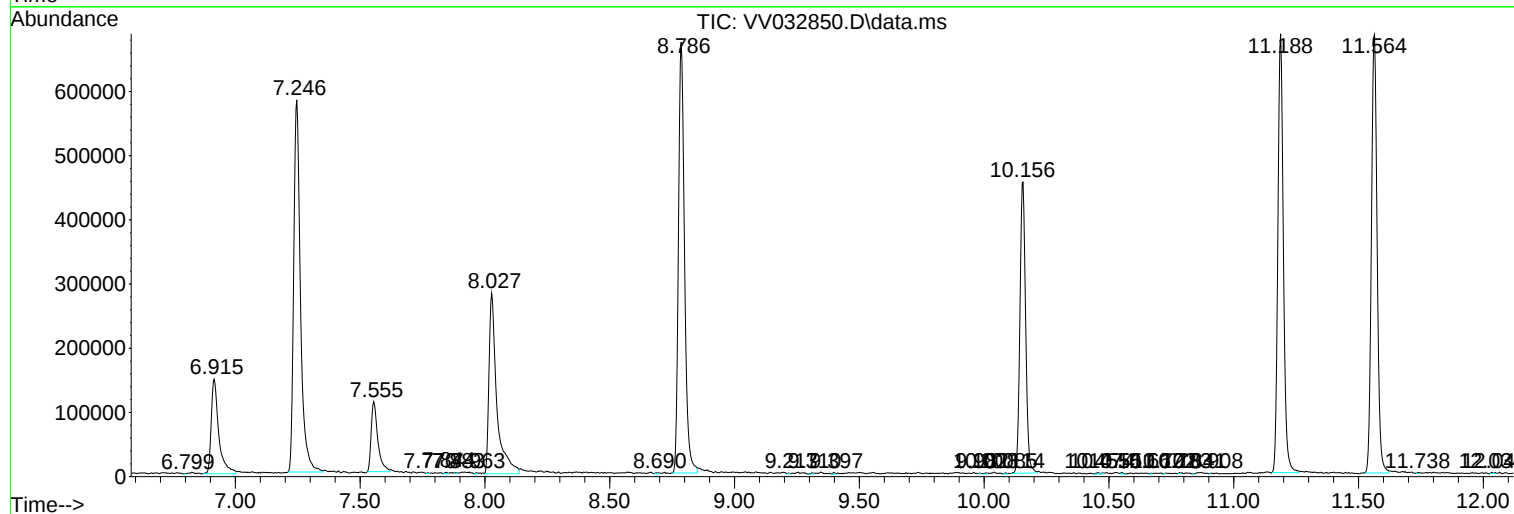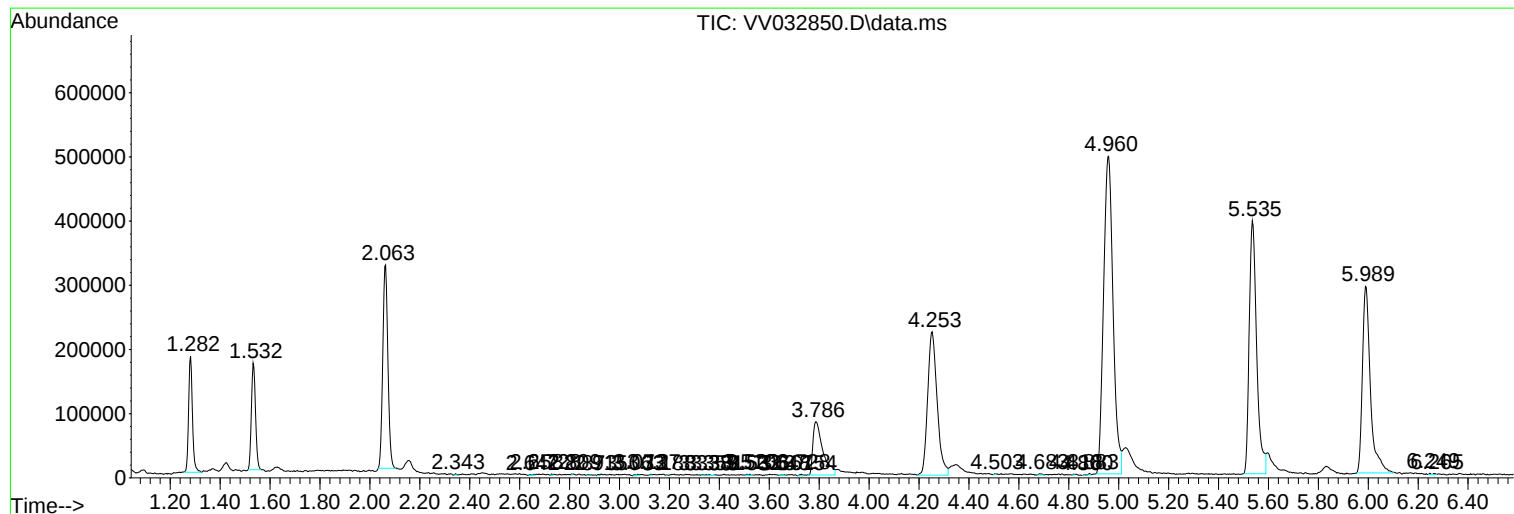

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032850.D
Acq On : 06 Nov 2023 13:23
Operator : SY/MD
Sample : VV1106WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032850.D
Acq On : 06 Nov 2023 13:23
Operator : SY/MD
Sample : VV1106WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------