

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032853.D
 Acq On : 06 Nov 2023 15:11
 Operator : SY/MD
 Sample : 05203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rBV	189878	195741	15.15%	1.869%
2	1.532	147	153	166	rVB	168617	194966	15.09%	1.862%
3	2.059	308	317	330	rBV	316089	450373	34.85%	4.301%
4	2.429	429	432	435	rBV5	1868	1696	0.13%	0.016%
5	2.445	435	437	443	rVB6	3123	2421	0.19%	0.023%
6	2.683	508	511	512	rBV2	997	614	0.05%	0.006%
7	2.690	512	513	517	rVV3	1513	972	0.08%	0.009%
8	2.741	525	529	532	rBV4	1451	1178	0.09%	0.011%
9	2.760	532	535	538	rVB5	1458	739	0.06%	0.007%
10	2.783	538	542	543	rBV4	1360	969	0.07%	0.009%
11	2.818	549	553	558	rBV7	1658	1500	0.12%	0.014%
12	2.931	584	588	590	rBV4	1622	1235	0.10%	0.012%
13	3.024	615	617	619	rVB3	1180	483	0.04%	0.005%
14	3.040	619	622	624	rBV4	1033	551	0.04%	0.005%
15	3.053	624	626	629	rVB4	1327	673	0.05%	0.006%
16	3.101	639	641	643	rBV3	1325	662	0.05%	0.006%
17	3.146	652	655	658	rBV5	1547	1266	0.10%	0.012%
18	3.214	674	676	679	rVB3	2184	1003	0.08%	0.010%
19	3.249	683	687	691	rBV7	1366	1237	0.10%	0.012%
20	3.355	716	720	725	rBV8	2395	2044	0.16%	0.020%
21	3.384	725	729	732	rBV7	1734	1350	0.10%	0.013%
22	3.420	738	740	742	rBV3	1683	989	0.08%	0.009%
23	3.481	757	759	764	rBV5	1832	1430	0.11%	0.014%
24	3.503	764	766	768	rVB3	1120	631	0.05%	0.006%
25	3.516	768	770	773	rBV4	861	560	0.04%	0.005%
26	3.580	784	790	793	rBV6	2817	2583	0.20%	0.025%
27	3.600	793	796	800	rBV6	1737	1226	0.09%	0.012%
28	3.635	800	807	809	rBV7	1767	2084	0.16%	0.020%
29	3.725	831	835	837	rBV5	1664	1202	0.09%	0.011%
30	3.786	844	854	881	rBV	76764	213448	16.52%	2.039%
31	4.146	964	966	969	rVB4	1772	952	0.07%	0.009%
32	4.249	984	998	1020	rBV2	214073	556606	43.07%	5.316%
33	4.558	1091	1094	1098	rBV5	1619	1309	0.10%	0.013%
34	4.696	1134	1137	1138	rBV3	1767	847	0.07%	0.008%
35	4.841	1181	1182	1184	rVB2	1540	472	0.04%	0.005%
36	4.857	1184	1187	1192	rBV6	1793	1804	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032853.D
 Acq On : 06 Nov 2023 15:11
 Operator : SY/MD
 Sample : 05203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.956	1202	1218	1235	rBV2	489940	1292336	100.00%	12.342%
38	5.439	1366	1368	1374	rVB7	2303	1926	0.15%	0.018%
39	5.471	1376	1378	1380	rBV3	1901	742	0.06%	0.007%
40	5.535	1387	1398	1413	rBV	384603	784628	60.71%	7.494%
41	5.989	1527	1539	1573	rBV	286427	655229	50.70%	6.258%
42	6.529	1705	1707	1710	rBV4	1436	747	0.06%	0.007%
43	6.567	1717	1719	1720	rBV2	1371	520	0.04%	0.005%
44	6.664	1747	1749	1750	rBV2	1588	767	0.06%	0.007%
45	6.821	1796	1798	1803	rBV6	1046	781	0.06%	0.007%
46	6.915	1817	1827	1855	rBV	144528	298771	23.12%	2.853%
47	7.082	1876	1879	1884	rBV6	1870	1747	0.14%	0.017%
48	7.243	1918	1929	1961	rBV	573145	1079276	83.51%	10.308%
49	7.554	2017	2026	2041	rBV	108544	203597	15.75%	1.944%
50	8.027	2164	2173	2206	rBV	252694	538895	41.70%	5.147%
51	8.683	2375	2377	2380	rBV4	2930	2035	0.16%	0.019%
52	8.712	2384	2386	2391	rVB5	1705	1261	0.10%	0.012%
53	8.786	2398	2409	2429	rBV	661593	1113584	86.17%	10.635%
54	9.053	2488	2492	2494	rBV5	2324	1701	0.13%	0.016%
55	9.159	2524	2525	2527	rBV2	1197	546	0.04%	0.005%
56	9.210	2539	2541	2542	rBV3	1488	569	0.04%	0.005%
57	9.352	2580	2585	2588	rBV6	2103	1833	0.14%	0.018%
58	9.654	2677	2679	2681	rBV3	1413	641	0.05%	0.006%
59	9.789	2720	2721	2722	rBV	1337	433	0.03%	0.004%
60	10.030	2794	2796	2800	rBV5	2237	1982	0.15%	0.019%
61	10.156	2824	2835	2855	rVB	435477	694598	53.75%	6.634%
62	10.307	2880	2882	2884	rVB2	2195	918	0.07%	0.009%
63	10.323	2884	2887	2889	rBV4	1898	1285	0.10%	0.012%
64	10.509	2942	2945	2947	rBV4	1708	1268	0.10%	0.012%
65	10.612	2975	2977	2978	rBV2	1356	479	0.04%	0.005%
66	10.728	3009	3013	3016	rBV5	2045	1236	0.10%	0.012%
67	10.898	3062	3066	3069	rBV6	2235	1649	0.13%	0.016%
68	10.959	3082	3085	3090	rBV7	1577	1480	0.11%	0.014%
69	10.992	3093	3095	3098	rBV3	948	689	0.05%	0.007%
70	11.043	3106	3111	3117	rBV10	2798	3276	0.25%	0.031%
71	11.130	3135	3138	3140	rBV4	1579	1263	0.10%	0.012%
72	11.188	3145	3156	3176	rBV	651406	1028421	79.58%	9.822%
73	11.339	3199	3203	3204	rBV3	1925	1331	0.10%	0.013%
74	11.564	3261	3273	3290	rBV	666108	1069290	82.74%	10.212%
75	12.088	3434	3436	3439	rVB4	2695	1469	0.11%	0.014%
76	12.194	3467	3469	3470	rBV2	1420	569	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032853.D
 Acq On : 06 Nov 2023 15:11
 Operator : SY/MD
 Sample : 05203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.300	3499	3502	3506	rBV5	1670	1312	0.10%	0.013%
78	12.500	3562	3564	3566	rBV3	995	496	0.04%	0.005%
79	12.638	3602	3607	3611	rBV6	2193	2566	0.20%	0.025%
80	12.660	3612	3614	3621	rVB7	1736	1800	0.14%	0.017%
81	12.705	3626	3628	3631	rBV4	2033	1266	0.10%	0.012%
82	12.811	3658	3661	3668	rVB9	2032	1632	0.13%	0.016%
83	12.837	3668	3669	3671	rBV2	1820	893	0.07%	0.009%
84	12.918	3691	3694	3695	rBV3	1210	526	0.04%	0.005%
85	13.101	3749	3751	3752	rBV2	1487	572	0.04%	0.005%
86	13.165	3769	3771	3774	rBV3	1269	840	0.06%	0.008%
87	13.319	3816	3819	3821	rBV4	1319	1011	0.08%	0.010%
88	13.368	3832	3834	3838	rBV4	1219	691	0.05%	0.007%
89	13.387	3838	3840	3841	rBV2	1650	670	0.05%	0.006%
90	13.445	3854	3858	3859	rBV3	3167	2001	0.15%	0.019%
91	13.593	3902	3904	3909	rBV6	1589	1536	0.12%	0.015%
92	13.647	3917	3921	3923	rBV5	1289	844	0.07%	0.008%
93	13.680	3927	3931	3936	rBV7	3084	3477	0.27%	0.033%
94	13.815	3971	3973	3974	rBV2	1756	874	0.07%	0.008%
95	13.991	4025	4028	4030	rBV4	1684	1062	0.08%	0.010%
96	14.191	4088	4090	4093	rBV3	1299	854	0.07%	0.008%
97	14.223	4097	4100	4103	rBV4	1208	902	0.07%	0.009%
98	14.474	4176	4178	4180	rBV3	2052	1174	0.09%	0.011%
99	14.876	4300	4303	4305	rBV4	1687	1014	0.08%	0.010%
100	15.519	4501	4503	4505	rBV2	2138	1121	0.09%	0.011%




Sum of corrected areas: 10470718

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032853.D
Acq On : 06 Nov 2023 15:11
Operator : SY/MD
Sample : 05203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

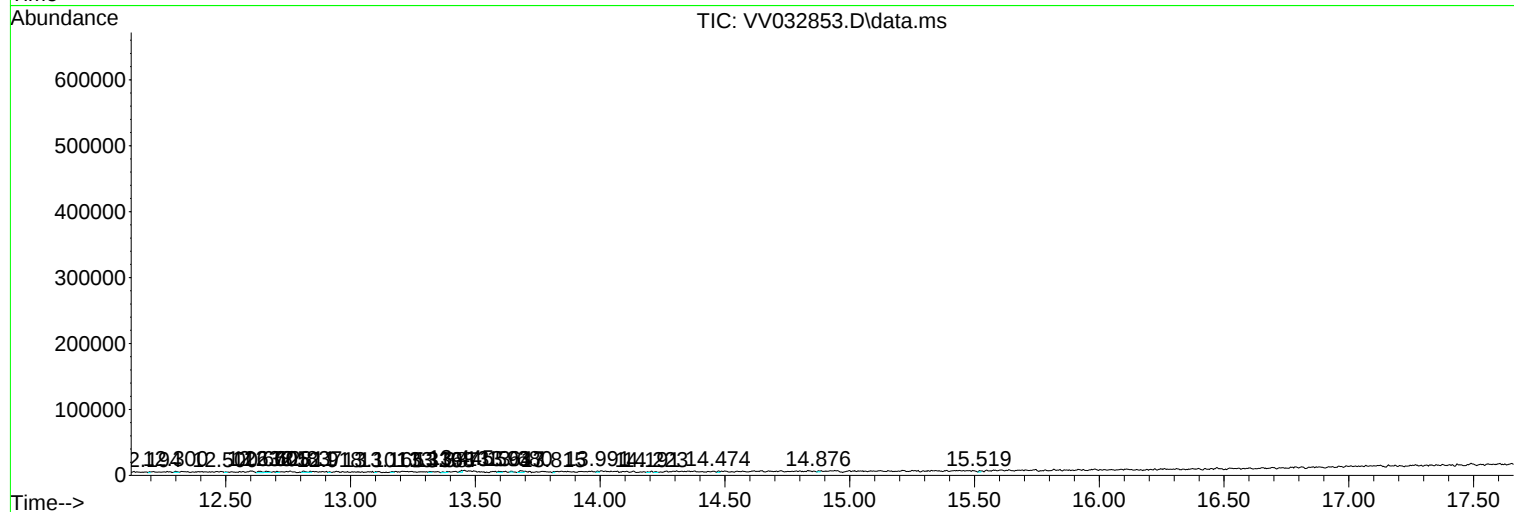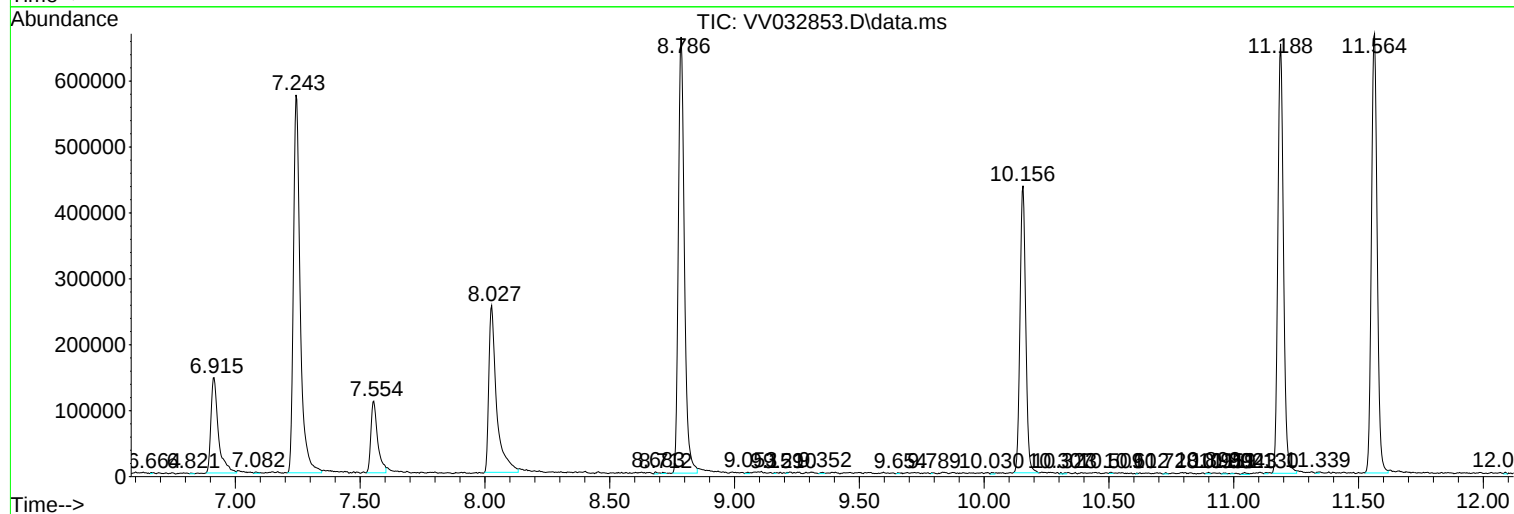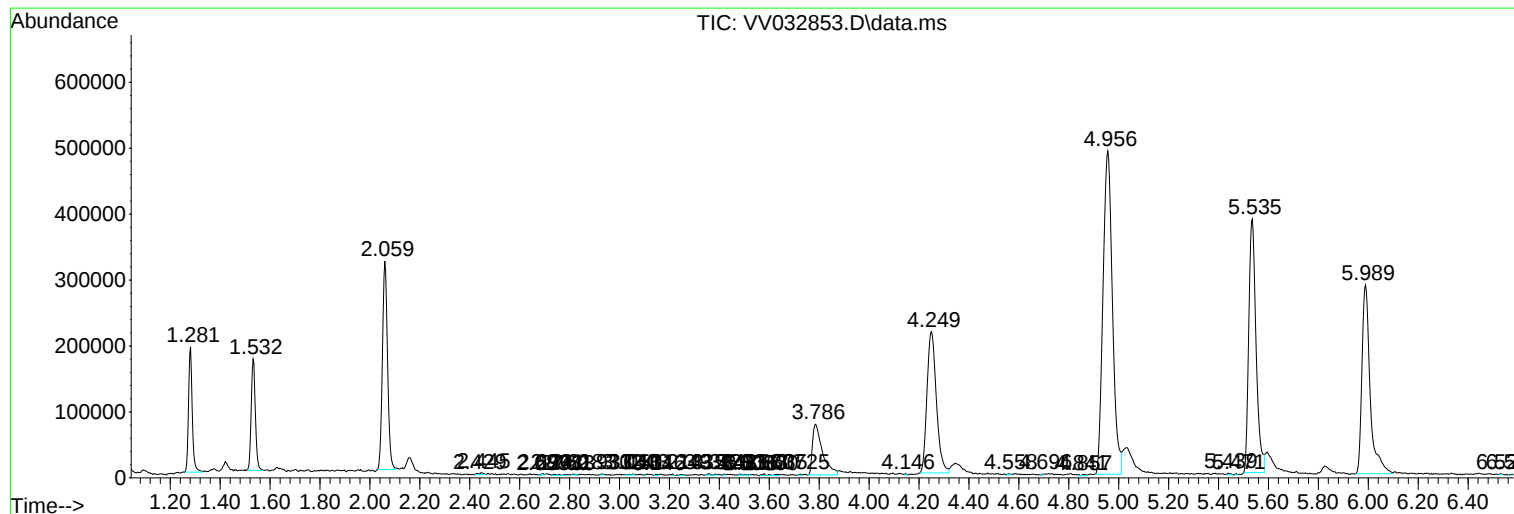

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032853.D
Acq On : 06 Nov 2023 15:11
Operator : SY/MD
Sample : 05203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032853.D
Acq On : 06 Nov 2023 15:11
Operator : SY/MD
Sample : 05203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------