

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032854.D
 Acq On : 06 Nov 2023 15:35
 Operator : SY/MD
 Sample : 05259-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rVB	165825	171993	13.97%	1.676%
2	1.532	147	153	168	rVB	158701	185178	15.04%	1.804%
3	2.059	309	317	332	rBV	289901	419868	34.11%	4.091%
4	2.397	418	422	425	rBV4	1660	1335	0.11%	0.013%
5	2.497	451	453	457	rVV6	1362	948	0.08%	0.009%
6	2.632	489	495	497	rBV7	1734	1697	0.14%	0.017%
7	2.770	536	538	542	rBV5	1305	1077	0.09%	0.010%
8	2.789	542	544	545	rBV2	1240	533	0.04%	0.005%
9	2.863	563	567	569	rBV5	1218	778	0.06%	0.008%
10	2.908	577	581	583	rBV5	1571	1170	0.10%	0.011%
11	2.992	605	607	608	rBV2	1199	577	0.05%	0.006%
12	3.024	615	617	620	rVB4	1202	683	0.06%	0.007%
13	3.040	620	622	625	rBV4	2159	1561	0.13%	0.015%
14	3.063	627	629	631	rBV3	995	504	0.04%	0.005%
15	3.104	638	642	646	rBV6	1411	1314	0.11%	0.013%
16	3.121	646	647	654	rVB6	1809	1478	0.12%	0.014%
17	3.166	655	661	663	rBV6	1640	1431	0.12%	0.014%
18	3.317	706	708	711	rBV3	859	470	0.04%	0.005%
19	3.378	723	727	733	rBV8	2674	2703	0.22%	0.026%
20	3.413	736	738	743	rVB5	1241	1144	0.09%	0.011%
21	3.542	776	778	783	rBV5	1273	1224	0.10%	0.012%
22	3.567	783	786	787	rBV3	1069	558	0.05%	0.005%
23	3.641	807	809	811	rBV3	1825	1019	0.08%	0.010%
24	3.725	830	835	836	rBV4	835	700	0.06%	0.007%
25	3.748	840	842	846	rBV3	1142	667	0.05%	0.006%
26	3.789	846	855	877	rBV	79787	215207	17.48%	2.097%
27	4.252	985	999	1020	rBV	204319	526509	42.77%	5.130%
28	4.503	1075	1077	1078	rBV2	1273	515	0.04%	0.005%
29	4.567	1095	1097	1100	rBV4	1423	983	0.08%	0.010%
30	4.651	1121	1123	1126	rVB3	2284	915	0.07%	0.009%
31	4.674	1126	1130	1131	rBV3	1805	1095	0.09%	0.011%
32	4.821	1170	1176	1180	rBV8	1602	1708	0.14%	0.017%
33	4.960	1202	1219	1235	rBV2	465326	1230942	100.00%	11.993%
34	5.352	1338	1341	1346	rBV8	1794	1660	0.13%	0.016%
35	5.487	1379	1383	1385	rBV4	1679	1049	0.09%	0.010%
36	5.535	1386	1398	1414	rBV	385425	807347	65.59%	7.866%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032854.D
 Acq On : 06 Nov 2023 15:35
 Operator : SY/MD
 Sample : 05259-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.989	1528	1539	1572	rBV	273256	618923	50.28%	6.030%
38	6.259	1621	1623	1625	rBV2	1806	1050	0.09%	0.010%
39	6.358	1651	1654	1656	rBV3	1804	1035	0.08%	0.010%
40	6.390	1662	1664	1666	rBV3	1407	675	0.05%	0.007%
41	6.503	1697	1699	1701	rBV3	1164	482	0.04%	0.005%
42	6.545	1709	1712	1713	rBV3	2210	1141	0.09%	0.011%
43	6.554	1713	1715	1718	rVV4	1950	1149	0.09%	0.011%
44	6.590	1722	1726	1728	rBV4	2334	1579	0.13%	0.015%
45	6.728	1768	1769	1776	rVB7	1417	1233	0.10%	0.012%
46	6.786	1786	1787	1790	rBV3	1203	654	0.05%	0.006%
47	6.802	1790	1792	1796	rBV5	1486	855	0.07%	0.008%
48	6.915	1816	1827	1845	rBV	139025	280428	22.78%	2.732%
49	7.181	1908	1910	1916	rBV6	1289	1189	0.10%	0.012%
50	7.246	1918	1930	1960	rBV	545498	1023035	83.11%	9.968%
51	7.519	2013	2015	2016	rBV2	1304	566	0.05%	0.006%
52	7.554	2018	2026	2053	rVV	104068	204609	16.62%	1.994%
53	7.966	2152	2154	2156	rBV2	1577	593	0.05%	0.006%
54	7.982	2157	2159	2161	rBV3	1758	938	0.08%	0.009%
55	8.027	2163	2173	2206	rBV	274878	584623	47.49%	5.696%
56	8.567	2339	2341	2347	rBV6	1588	1402	0.11%	0.014%
57	8.670	2368	2373	2379	rBV7	1498	2092	0.17%	0.020%
58	8.786	2396	2409	2438	rBV	670801	1148914	93.34%	11.194%
59	9.287	2562	2565	2567	rBV4	2110	1389	0.11%	0.014%
60	9.378	2591	2593	2595	rBV3	1178	618	0.05%	0.006%
61	9.471	2620	2622	2625	rBV3	2287	1009	0.08%	0.010%
62	9.551	2644	2647	2651	rBV5	1730	1535	0.12%	0.015%
63	9.815	2726	2729	2730	rBV3	1141	788	0.06%	0.008%
64	10.043	2795	2800	2803	rVV6	1890	1659	0.13%	0.016%
65	10.085	2811	2813	2816	rVB3	1251	488	0.04%	0.005%
66	10.101	2816	2818	2821	rBV3	1393	760	0.06%	0.007%
67	10.156	2823	2835	2850	rBV	438311	697143	56.63%	6.792%
68	10.316	2878	2885	2887	rBV7	3154	2945	0.24%	0.029%
69	10.625	2978	2981	2984	rBV5	1701	1007	0.08%	0.010%
70	10.770	3024	3026	3028	rBV3	1491	709	0.06%	0.007%
71	10.815	3037	3040	3044	rBV6	1139	921	0.07%	0.009%
72	10.834	3044	3046	3047	rBV2	1482	525	0.04%	0.005%
73	10.966	3084	3087	3089	rBV4	1446	1025	0.08%	0.010%
74	11.008	3098	3100	3102	rVB3	1451	430	0.03%	0.004%
75	11.059	3114	3116	3123	rBV6	1339	1224	0.10%	0.012%
76	11.188	3145	3156	3176	rBV	665300	1035468	84.12%	10.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032854.D
 Acq On : 06 Nov 2023 15:35
 Operator : SY/MD
 Sample : 05259-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.503	3250	3254	3257	rBV5	1490	1424	0.12%	0.014%
78	11.564	3261	3273	3289	rBV	642510	1022435	83.06%	9.962%
79	12.300	3497	3502	3503	rBV4	1558	1505	0.12%	0.015%
80	12.358	3517	3520	3523	rBV3	2447	2001	0.16%	0.019%
81	12.522	3567	3571	3573	rBV3	1972	1336	0.11%	0.013%
82	12.979	3711	3713	3715	rBV4	1294	836	0.07%	0.008%
83	13.024	3725	3727	3730	rBV3	1589	1166	0.09%	0.011%
84	13.133	3759	3761	3762	rBV2	970	458	0.04%	0.004%
85	13.159	3767	3769	3774	rVB5	2233	1404	0.11%	0.014%
86	13.329	3819	3822	3823	rBV3	1081	554	0.05%	0.005%
87	13.371	3832	3835	3838	rBV5	2415	1589	0.13%	0.015%
88	13.500	3874	3875	3880	rVB5	2199	1057	0.09%	0.010%
89	13.522	3880	3882	3886	rBV5	1241	885	0.07%	0.009%
90	13.580	3898	3900	3903	rBV3	1387	1063	0.09%	0.010%
91	13.657	3919	3924	3927	rBV7	1888	1625	0.13%	0.016%
92	13.680	3929	3931	3933	rBV3	1811	828	0.07%	0.008%
93	13.956	4014	4017	4021	rVB5	1494	1339	0.11%	0.013%
94	14.020	4034	4037	4039	rBV4	1238	831	0.07%	0.008%
95	14.255	4108	4110	4111	rBV2	1998	693	0.06%	0.007%
96	14.580	4209	4211	4213	rBV3	1495	599	0.05%	0.006%
97	14.840	4290	4292	4295	rBV4	1837	956	0.08%	0.009%
98	14.892	4303	4308	4311	rBV7	1872	2254	0.18%	0.022%
99	14.934	4318	4321	4322	rBV3	1463	795	0.06%	0.008%
100	14.963	4328	4330	4331	rBV2	1732	680	0.06%	0.007%




Sum of corrected areas: 10263661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032854.D
Acq On : 06 Nov 2023 15:35
Operator : SY/MD
Sample : 05259-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

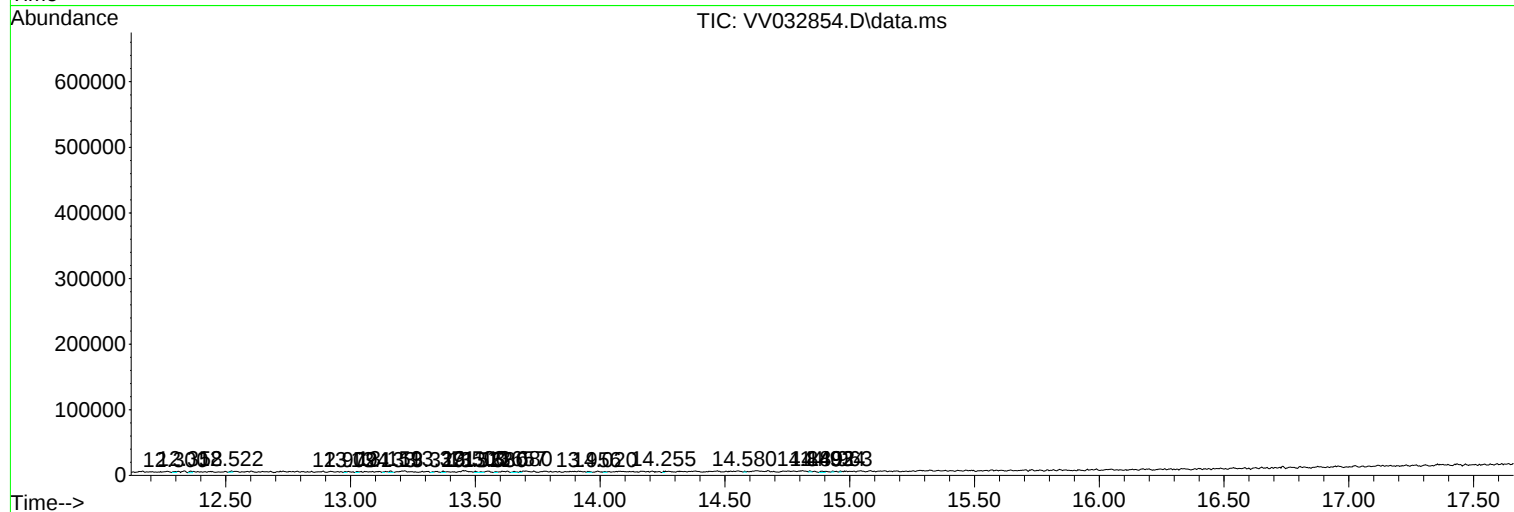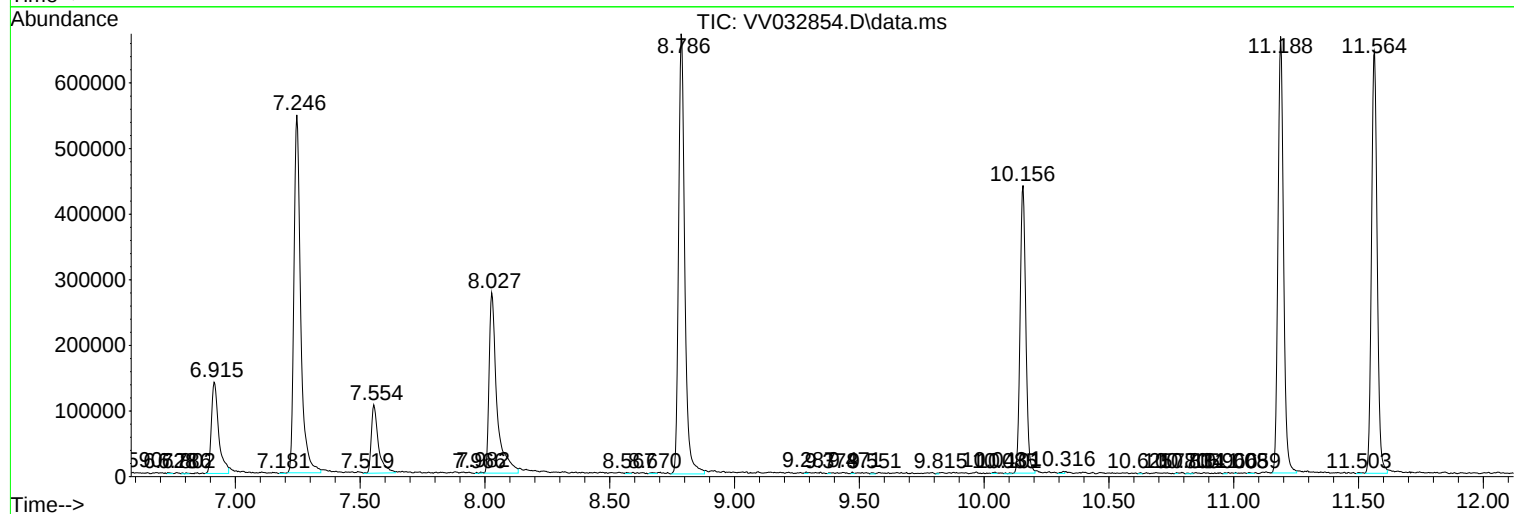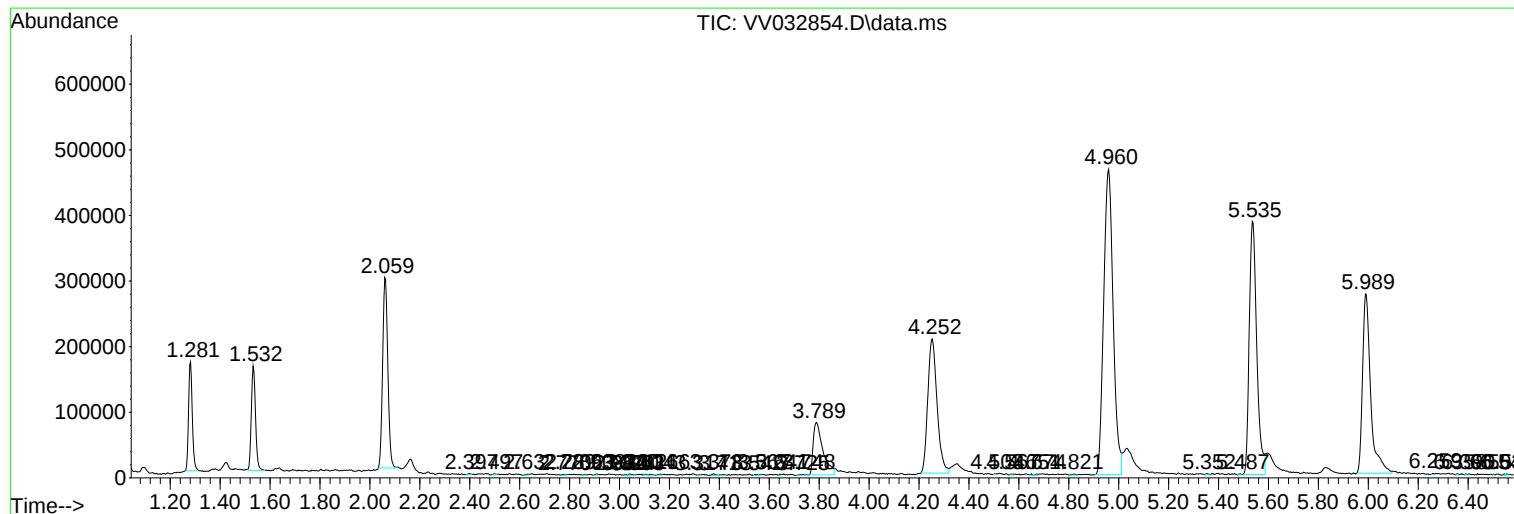

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032854.D
Acq On : 06 Nov 2023 15:35
Operator : SY/MD
Sample : 05259-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032854.D
Acq On : 06 Nov 2023 15:35
Operator : SY/MD
Sample : 05259-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------