

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032857.D
 Acq On : 06 Nov 2023 16:45
 Operator : SY/MD
 Sample : VIBLK240
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rBV	148507	159354	13.04%	1.580%
2	1.532	147	153	168	rVB	149997	173691	14.22%	1.722%
3	2.059	309	317	331	rBV	255806	375115	30.70%	3.719%
4	2.876	566	571	574	rVV7	1150	1091	0.09%	0.011%
5	2.931	586	588	591	rBV4	1694	1158	0.09%	0.011%
6	2.963	595	598	602	rVV6	1460	983	0.08%	0.010%
7	2.998	608	609	612	rBV4	1225	723	0.06%	0.007%
8	3.024	612	617	618	rBV6	1218	1069	0.09%	0.011%
9	3.092	636	638	641	rVB4	1566	967	0.08%	0.010%
10	3.114	641	645	646	rBV4	1425	1052	0.09%	0.010%
11	3.198	669	671	673	rBV3	1153	749	0.06%	0.007%
12	3.262	687	691	694	rBV6	2012	1796	0.15%	0.018%
13	3.326	709	711	716	rVB6	2126	1619	0.13%	0.016%
14	3.352	716	719	721	rVB4	1444	663	0.05%	0.007%
15	3.468	753	755	758	rBV3	1325	938	0.08%	0.009%
16	3.651	809	812	817	rVB7	1949	1698	0.14%	0.017%
17	3.674	817	819	824	rBV7	1474	1410	0.12%	0.014%
18	3.722	831	834	836	rBV5	1447	877	0.07%	0.009%
19	3.789	844	855	882	rBV2	94310	265367	21.72%	2.631%
20	4.252	987	999	1021	rBV	195427	486334	39.80%	4.821%
21	4.500	1073	1076	1079	rBV5	2169	1995	0.16%	0.020%
22	4.638	1116	1119	1121	rBV4	2437	1508	0.12%	0.015%
23	4.889	1196	1197	1201	rBV3	1429	988	0.08%	0.010%
24	4.960	1203	1219	1236	rBV2	460023	1221801	100.00%	12.113%
25	5.474	1376	1379	1380	rBV3	1420	798	0.07%	0.008%
26	5.538	1386	1399	1414	rBV	354000	723954	59.25%	7.177%
27	5.992	1528	1540	1556	rBV	274139	578823	47.37%	5.738%
28	6.362	1653	1655	1657	rBV3	2047	898	0.07%	0.009%
29	6.558	1713	1716	1718	rVB4	1844	925	0.08%	0.009%
30	6.657	1743	1747	1748	rBV4	1256	885	0.07%	0.009%
31	6.699	1756	1760	1761	rBV3	1349	893	0.07%	0.009%
32	6.754	1775	1777	1781	rVB5	2197	1368	0.11%	0.014%
33	6.773	1781	1783	1786	rBV4	1213	774	0.06%	0.008%
34	6.831	1799	1801	1806	rVB4	2568	1978	0.16%	0.020%
35	6.850	1806	1807	1809	rBV2	1579	701	0.06%	0.007%
36	6.915	1818	1827	1850	rBV	140244	285940	23.40%	2.835%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032857.D
 Acq On : 06 Nov 2023 16:45
 Operator : SY/MD
 Sample : VIBLK240
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	7.246	1919	1930	1964	rBV	512877	971896	79.55%	9.635%
38	7.554	2018	2026	2047	rBV	105703	205780	16.84%	2.040%
39	7.709	2071	2074	2077	rBV5	2381	1557	0.13%	0.015%
40	7.857	2115	2120	2121	rBV4	1673	1136	0.09%	0.011%
41	7.876	2125	2126	2128	rBV2	1274	704	0.06%	0.007%
42	8.027	2164	2173	2210	rBV	303823	650217	53.22%	6.446%
43	8.452	2302	2305	2308	rBV5	1276	962	0.08%	0.010%
44	8.603	2347	2352	2353	rBV5	1210	1067	0.09%	0.011%
45	8.661	2366	2370	2373	rBV6	1955	1689	0.14%	0.017%
46	8.786	2399	2409	2436	rBV	594934	1020970	83.56%	10.122%
47	9.037	2485	2487	2491	rBV5	2028	982	0.08%	0.010%
48	9.175	2527	2530	2534	rBV6	2641	1776	0.15%	0.018%
49	9.197	2534	2537	2540	rBV3	2754	1839	0.15%	0.018%
50	9.239	2546	2550	2555	rBV7	1532	1462	0.12%	0.014%
51	9.271	2555	2560	2563	rVV6	1812	1438	0.12%	0.014%
52	9.808	2724	2727	2731	rBV5	1185	1153	0.09%	0.011%
53	9.844	2735	2738	2741	rVV5	1236	787	0.06%	0.008%
54	9.873	2741	2747	2756	rVV8	6897	10996	0.90%	0.109%
55	9.918	2759	2761	2763	rVB3	2175	996	0.08%	0.010%
56	9.953	2769	2772	2773	rBV3	1366	710	0.06%	0.007%
57	10.024	2787	2794	2796	rBV8	1960	1800	0.15%	0.018%
58	10.156	2824	2835	2849	rBV	456896	720606	58.98%	7.144%
59	10.323	2885	2887	2890	rBV4	1658	809	0.07%	0.008%
60	10.368	2899	2901	2905	rVB5	1708	1109	0.09%	0.011%
61	10.484	2930	2937	2944	rBV9	5984	10277	0.84%	0.102%
62	10.574	2963	2965	2969	rVB4	2918	2170	0.18%	0.022%
63	10.596	2969	2972	2976	rBV6	2192	2084	0.17%	0.021%
64	10.660	2991	2992	2995	rVV3	1534	862	0.07%	0.009%
65	10.686	2998	3000	3006	rVB5	1997	1631	0.13%	0.016%
66	10.959	3080	3085	3088	rVB6	1448	1267	0.10%	0.013%
67	10.976	3088	3090	3093	rBV4	1055	759	0.06%	0.008%
68	11.017	3099	3103	3106	rBV5	2493	1781	0.15%	0.018%
69	11.037	3106	3109	3115	rVB8	1594	1760	0.14%	0.017%
70	11.188	3146	3156	3179	rVB	594694	930498	76.16%	9.225%
71	11.307	3191	3193	3195	rBV3	2694	1019	0.08%	0.010%
72	11.564	3261	3273	3292	rBV	602144	977833	80.03%	9.694%
73	11.744	3323	3329	3330	rBV7	1820	1823	0.15%	0.018%
74	11.844	3357	3360	3364	rVB5	1759	1303	0.11%	0.013%
75	11.869	3364	3368	3372	rBV6	1528	1301	0.11%	0.013%
76	11.918	3380	3383	3389	rBV6	1632	1469	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
 Data File : VV032857.D
 Acq On : 06 Nov 2023 16:45
 Operator : SY/MD
 Sample : VIBLK240
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK240

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.069	3427	3430	3435	rBV6	1927	1618	0.13%	0.016%
78	12.114	3442	3444	3449	rVB6	1210	827	0.07%	0.008%
79	12.149	3449	3455	3459	rBV8	1750	1966	0.16%	0.019%
80	12.249	3483	3486	3488	rBV3	1770	951	0.08%	0.009%
81	12.278	3492	3495	3498	rBV5	1292	1095	0.09%	0.011%
82	12.310	3501	3505	3507	rBV5	1646	1094	0.09%	0.011%
83	12.590	3586	3592	3603	rVB4	16117	23458	1.92%	0.233%
84	12.657	3609	3613	3615	rBV5	1325	845	0.07%	0.008%
85	12.686	3620	3622	3625	rVB4	2166	1033	0.08%	0.010%
86	12.709	3625	3629	3630	rBV4	1371	732	0.06%	0.007%
87	12.828	3664	3666	3669	rBV4	1900	1122	0.09%	0.011%
88	12.853	3669	3674	3678	rVV8	1884	2571	0.21%	0.025%
89	13.101	3749	3751	3756	rBV6	1737	1278	0.10%	0.013%
90	13.130	3756	3760	3762	rBV4	874	745	0.06%	0.007%
91	13.204	3774	3783	3792	rBV3	23314	38202	3.13%	0.379%
92	13.291	3808	3810	3812	rVV3	1528	676	0.06%	0.007%
93	13.442	3848	3857	3871	rBV	61808	102811	8.41%	1.019%
94	13.593	3902	3904	3906	rBV3	1491	686	0.06%	0.007%
95	13.612	3906	3910	3913	rVV5	1490	1318	0.11%	0.013%
96	13.686	3924	3933	3945	rVB	33595	56097	4.59%	0.556%
97	14.172	4081	4084	4089	rBV7	1971	2158	0.18%	0.021%
98	14.207	4089	4095	4097	rVV6	2481	2078	0.17%	0.021%
99	15.107	4371	4375	4379	rBV6	1842	1351	0.11%	0.013%
100	15.339	4445	4447	4449	rBV3	1757	949	0.08%	0.009%




Sum of corrected areas: 10086822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032857.D
Acq On : 06 Nov 2023 16:45
Operator : SY/MD
Sample : VIBLK240
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

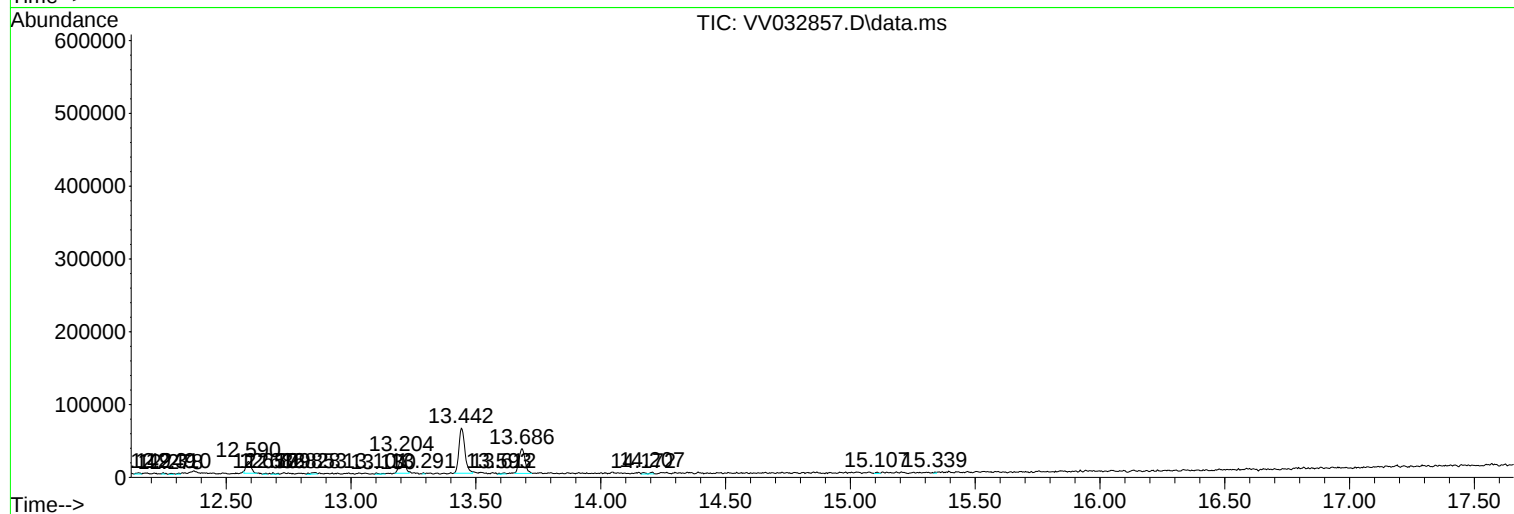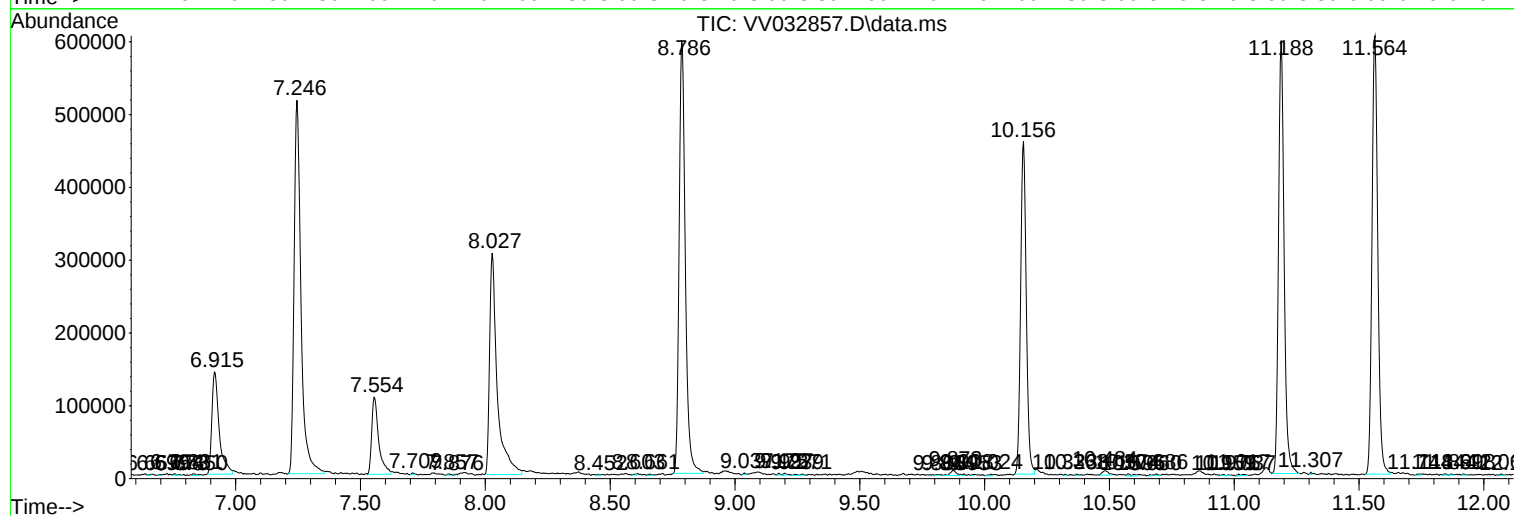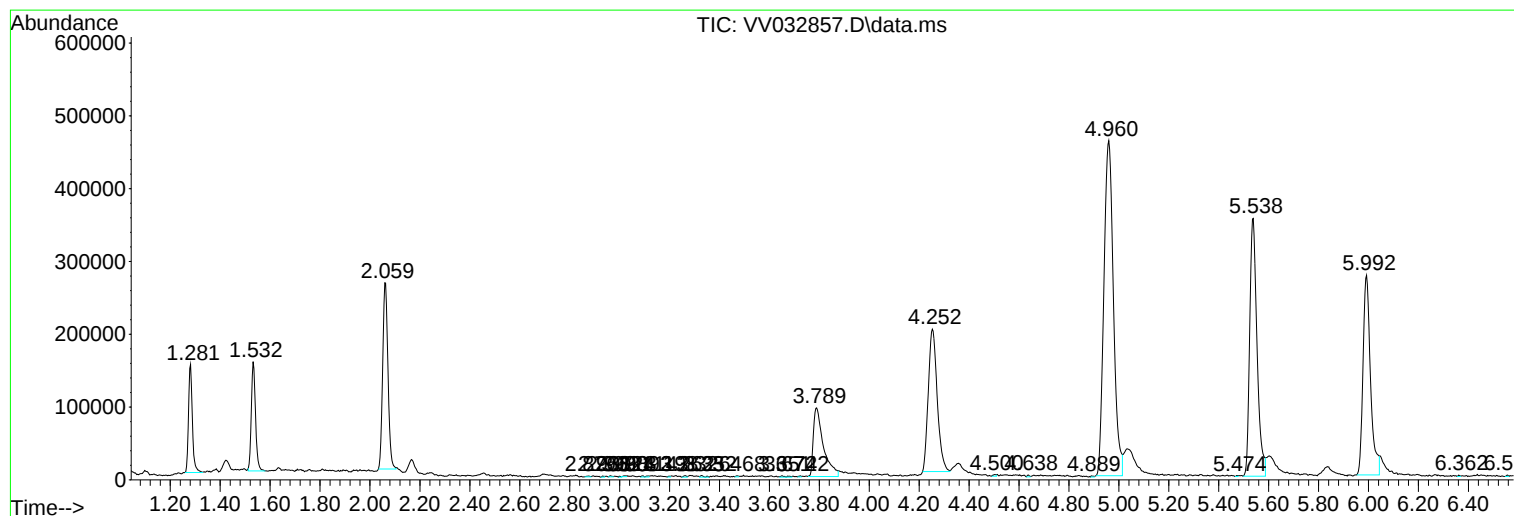

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032857.D
Acq On : 06 Nov 2023 16:45
Operator : SY/MD
Sample : VIBLK240
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032857.D
Acq On : 06 Nov 2023 16:45
Operator : SY/MD
Sample : VIBLK240
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------