


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110623\
Data File : VV032848.D
Acq On : 06 Nov 2023 11:46
Operator : SY/MD
Sample : BFB228
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB228

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Title : VOC Analysis
Last Update : Tue Nov 07 01:35:20 2023

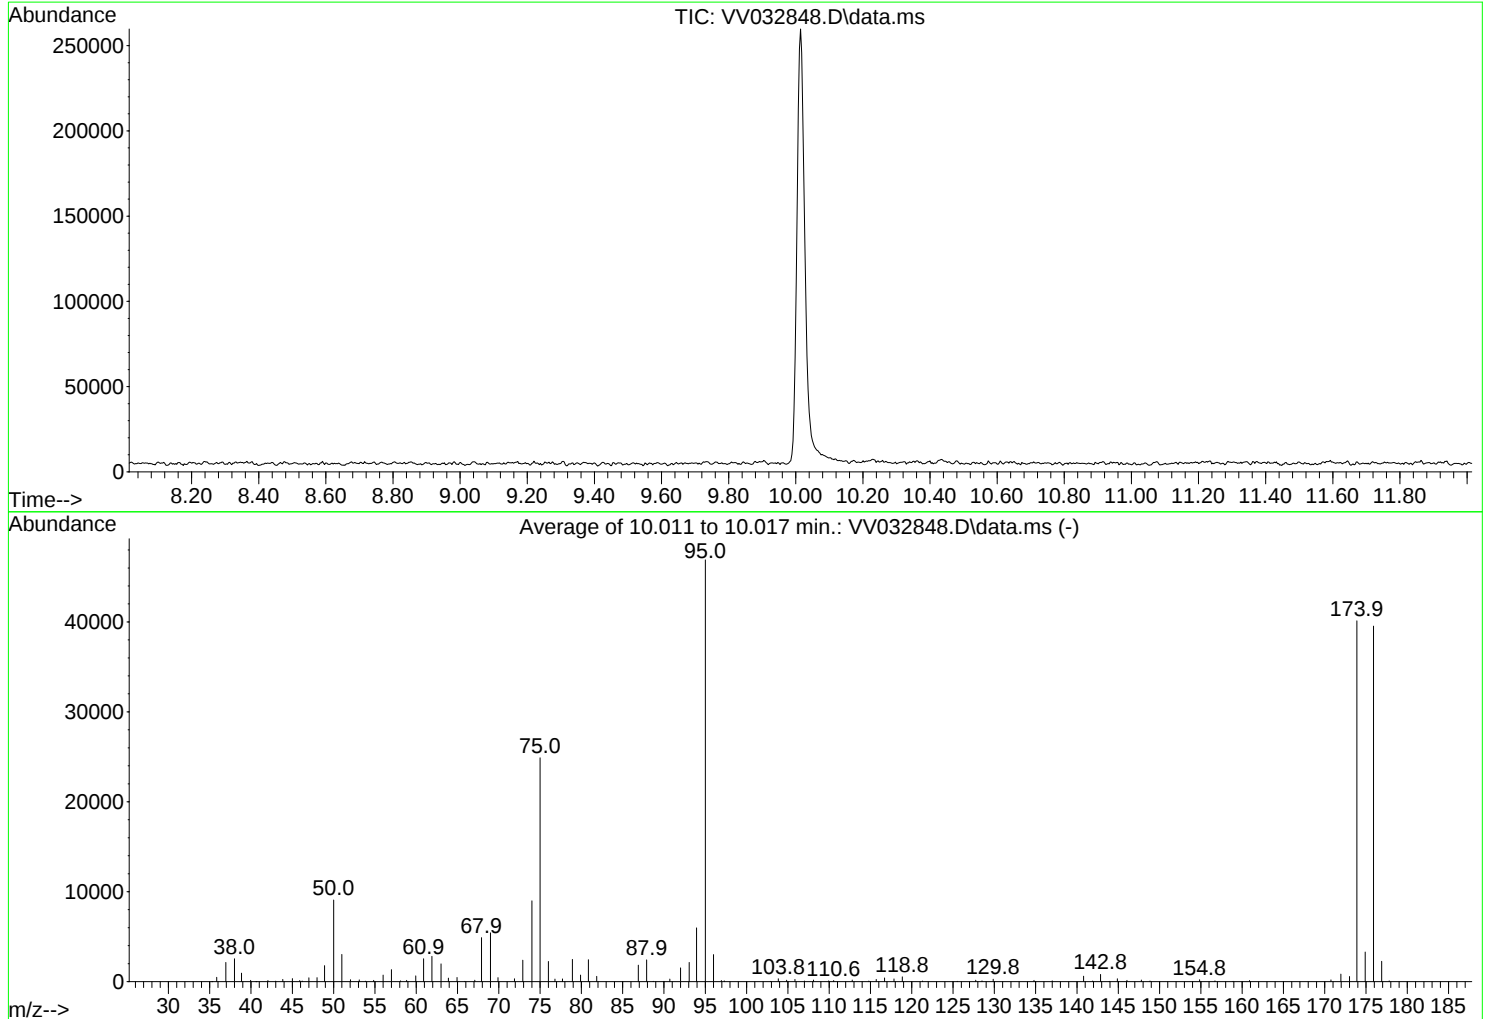

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	9075	PASS
75	95	30	80	53.1	24899	PASS
95	95	100	100	100.0	46904	PASS
96	95	5	9	6.4	3013	PASS
173	174	0.00	2	1.4	568	PASS
174	95	50	120	85.5	40117	PASS
175	174	5	9	8.2	3292	PASS
176	174	95	105	98.5	39531	PASS
177	176	5	10	5.7	2267	PASS

m/z	Abundance
35.40	156.0
36.20	152.0
36.80	184.0
37.60	131.0
38.70	206.0
39.90	226.0
40.50	178.0
41.40	138.0
41.60	138.0
42.90	156.0
43.90	507.0
45.20	126.0
46.60	118.0
47.20	157.0
48.90	120.0
49.70	115.0
51.30	120.0
52.90	105.0
53.80	105.0
54.80	180.0
57.10	101.0
57.70	109.0
58.20	101.0
63.20	102.0
67.30	124.0
71.90	159.0
73.60	117.0
75.30	143.0
76.90	103.0
79.40	121.0
81.50	107.0
84.20	104.0
129.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.20	135.0
35.90	453.0
37.00	2335.0
38.00	2479.0
38.90	1230.0
40.00	368.0
40.70	193.0
42.10	139.0
42.80	178.0
43.80	765.0
45.00	538.0
45.90	170.0
47.00	588.0
48.00	423.0
48.90	1849.0
50.00	9055.0
51.00	3000.0
52.00	214.0
52.90	185.0
53.10	184.0
53.90	156.0
54.90	348.0
56.00	696.0
57.00	1455.0
58.00	189.0
58.80	148.0
59.90	552.0
60.90	2486.0
61.90	2760.0
63.00	2248.0
63.90	412.0
65.00	447.0
65.90	128.0
67.00	280.0
67.90	5085.0
69.00	5411.0
69.90	462.0
71.90	433.0
72.90	2430.0
74.00	8783.0
75.00	24600.0
76.00	2457.0
76.80	384.0
77.70	376.0
78.90	2497.0
79.90	736.0
80.80	2286.0
81.80	663.0
86.90	1728.0
87.90	2554.0
88.70	123.0
90.70	288.0
92.00	1401.0
93.00	1945.0
93.90	6024.0
95.00	46568.0
96.00	3015.0
96.90	115.0
97.30	123.0
102.90	102.0
103.90	315.0
104.80	150.0
105.80	233.0
108.10	165.0
110.70	135.0
112.80	178.0
114.80	126.0
115.70	188.0
116.60	378.0
117.80	293.0
118.90	486.0
121.30	114.0
125.50	111.0
127.80	180.0
128.50	139.0
129.90	219.0
134.80	173.0
137.00	148.0
140.80	571.0
141.90	109.0
142.80	819.0
143.90	133.0
144.90	343.0
146.10	136.0
147.80	146.0
154.80	254.0
158.90	103.0
161.00	129.0
170.70	229.0
172.00	757.0
173.90	39136.0
174.90	3253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

175.9038544.0

176.902232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.20	156.0
35.80	481.0
37.00	2380.0
38.00	2706.0
38.90	1180.0
40.00	391.0
40.70	191.0
42.00	140.0
42.80	161.0
43.90	764.0
45.00	464.0
45.90	201.0
47.00	607.0
48.00	451.0
48.90	1901.0
50.00	9362.0
51.00	3120.0
52.10	215.0
53.10	200.0
53.90	162.0
54.90	344.0
56.00	751.0
57.00	1499.0
58.00	199.0
58.90	154.0
60.00	659.0
60.90	2634.0
61.90	2937.0
63.00	2161.0
63.90	396.0
65.00	489.0
67.00	296.0
67.90	4968.0
69.00	5646.0
69.90	457.0
71.90	500.0
72.90	2495.0
74.00	9354.0
75.00	25864.0
76.00	2312.0
76.80	429.0
77.70	301.0
78.90	2577.0
79.90	753.0
80.80	2518.0
81.80	586.0
86.90	1850.0
87.90	2521.0
90.70	311.0
92.00	1565.0
93.10	2185.0
93.90	6164.0
95.00	48400.0
96.00	3125.0
97.00	141.0
97.30	128.0
103.80	335.0
104.90	169.0
105.90	250.0
107.00	120.0
108.10	197.0
109.90	120.0
110.50	118.0
112.80	188.0
114.80	114.0
115.70	257.0
116.70	408.0
117.90	290.0
118.80	548.0
121.30	120.0
127.80	165.0
128.50	128.0
129.90	290.0
134.80	140.0
137.00	106.0
140.80	636.0
141.90	100.0
142.90	825.0
144.90	309.0
146.10	141.0
147.80	200.0
148.80	110.0
154.80	199.0
156.70	122.0
160.90	124.0
170.70	202.0
171.90	885.0
173.00	818.0
173.90	41280.0
174.90	3451.0
175.90	40896.0
176.90	2352.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

177.80

135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.20	190.0
35.80	530.0
37.00	2237.0
38.00	2467.0
38.90	1061.0
40.00	334.0
40.70	175.0
41.30	103.0
42.00	121.0
43.00	162.0
43.90	738.0
45.00	408.0
46.20	232.0
47.00	546.0
48.00	443.0
48.90	1939.0
50.00	8807.0
51.00	2973.0
52.10	232.0
53.10	200.0
53.90	172.0
54.90	268.0
56.00	755.0
57.00	1344.0
58.10	166.0
58.90	115.0
60.00	706.0
60.90	2530.0
61.90	2742.0
63.00	1837.0
63.90	351.0
64.90	472.0
67.10	289.0
67.90	4608.0
69.00	5206.0
69.90	408.0
71.90	489.0
72.90	2230.0
74.00	8818.0
75.00	24232.0
76.00	1945.0
76.80	380.0
77.60	211.0
78.90	2325.0
79.90	709.0
80.90	2493.0
81.90	525.0
86.90	1927.0
87.90	2172.0
90.00	100.0
90.70	261.0
92.00	1612.0
93.00	2276.0
94.00	5739.0
95.00	45744.0
96.00	2899.0
97.00	144.0
103.80	300.0
104.90	155.0
105.90	262.0
107.00	115.0
108.10	163.0
110.00	141.0
110.50	141.0
112.80	149.0
115.70	299.0
116.80	431.0
117.90	310.0
118.80	572.0
127.70	150.0
128.80	100.0
129.80	286.0
134.80	111.0
140.80	586.0
142.80	776.0
144.90	286.0
146.00	124.0
147.80	196.0
148.90	120.0
154.90	167.0
156.70	147.0
160.80	113.0
170.80	144.0
171.90	887.0
173.00	887.0
173.90	39936.0
174.90	3171.0
175.90	39152.0
176.90	2217.0
177.80	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228