




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037934.D
Acq On : 06 Nov 2024 17:34
Operator : SY/MD
Sample : P4714-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH9

Manual IntegrationsAPPROVED

Quant Time: Nov 06 22:47:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 22:44:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/07/2024
Supervised By :Semsettin Yesilyurt 11/07/2024

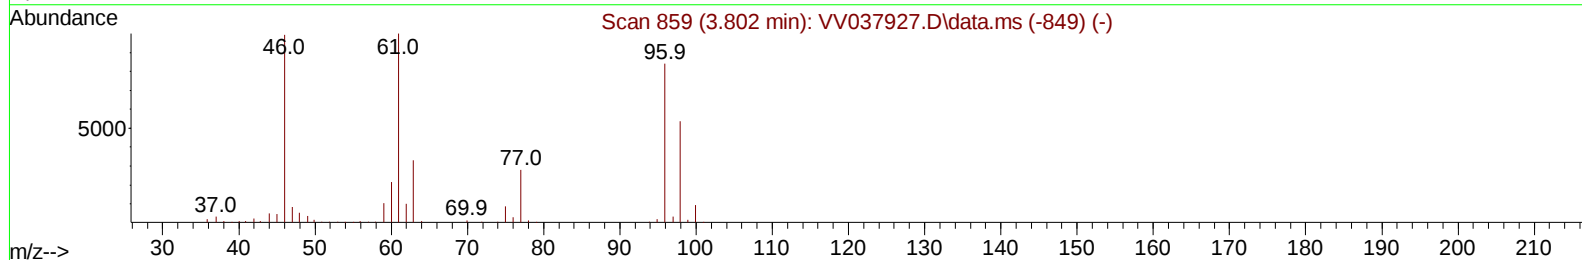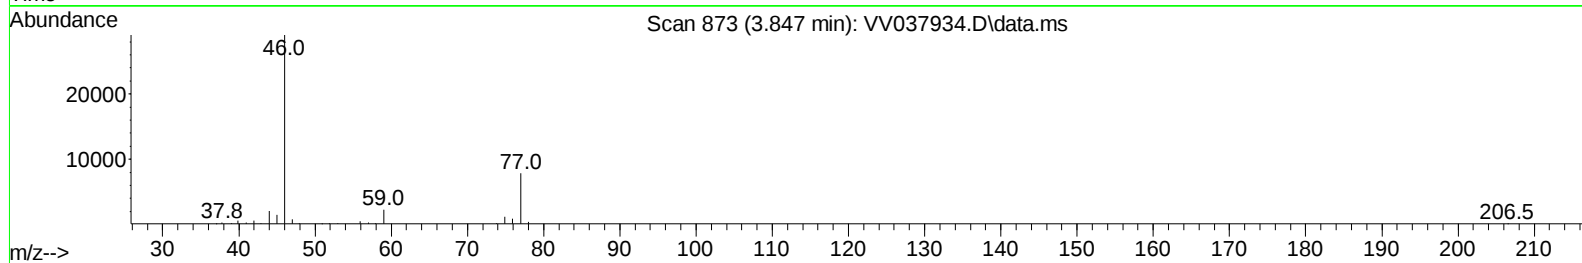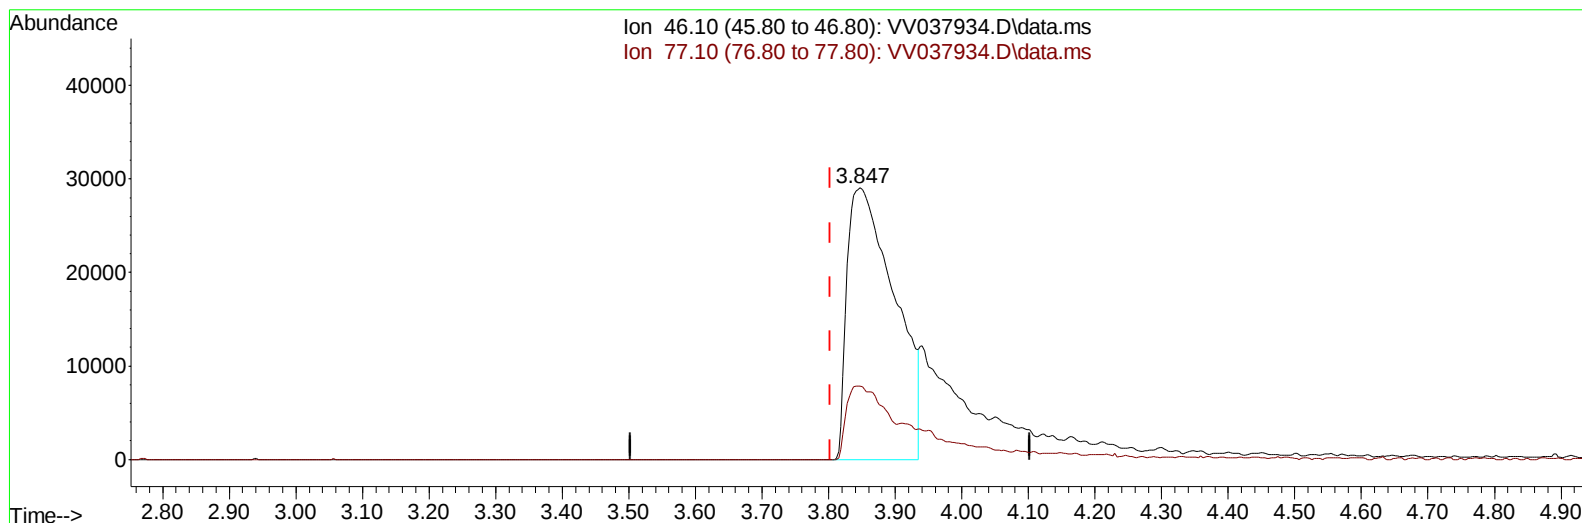

TIC: VV037934.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.045) 35.12 ug/L

response 143752

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	26.30	21.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037934.D
Acq On : 06 Nov 2024 17:34
Operator : SY/MD
Sample : P4714-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH9

Manual IntegrationsAPPROVED

Quant Time: Nov 06 22:47:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 22:44:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/07/2024
Supervised By :Semsettin Yesilyurt 11/07/2024

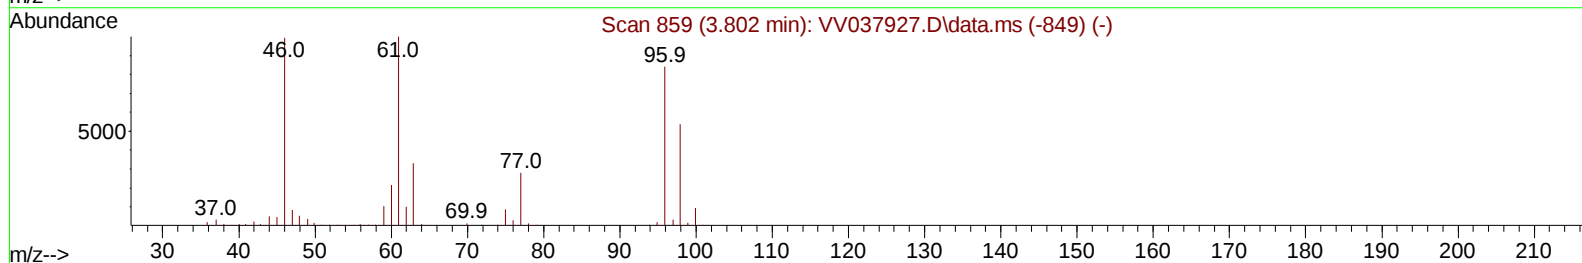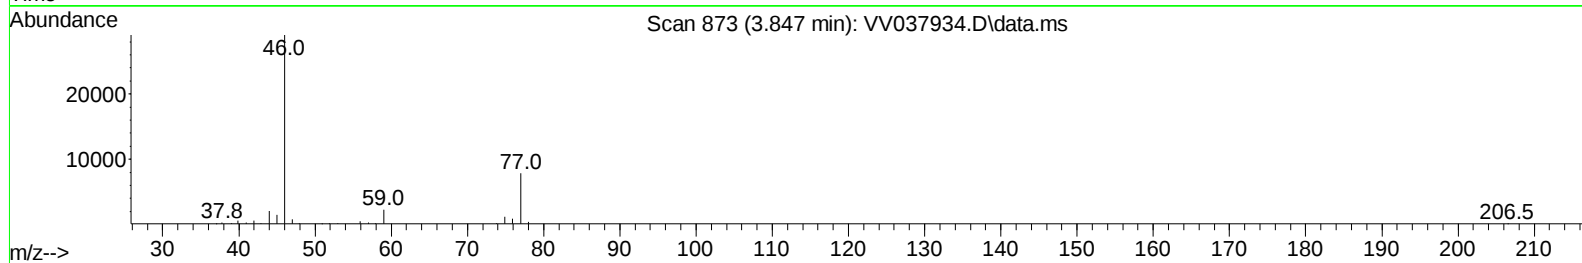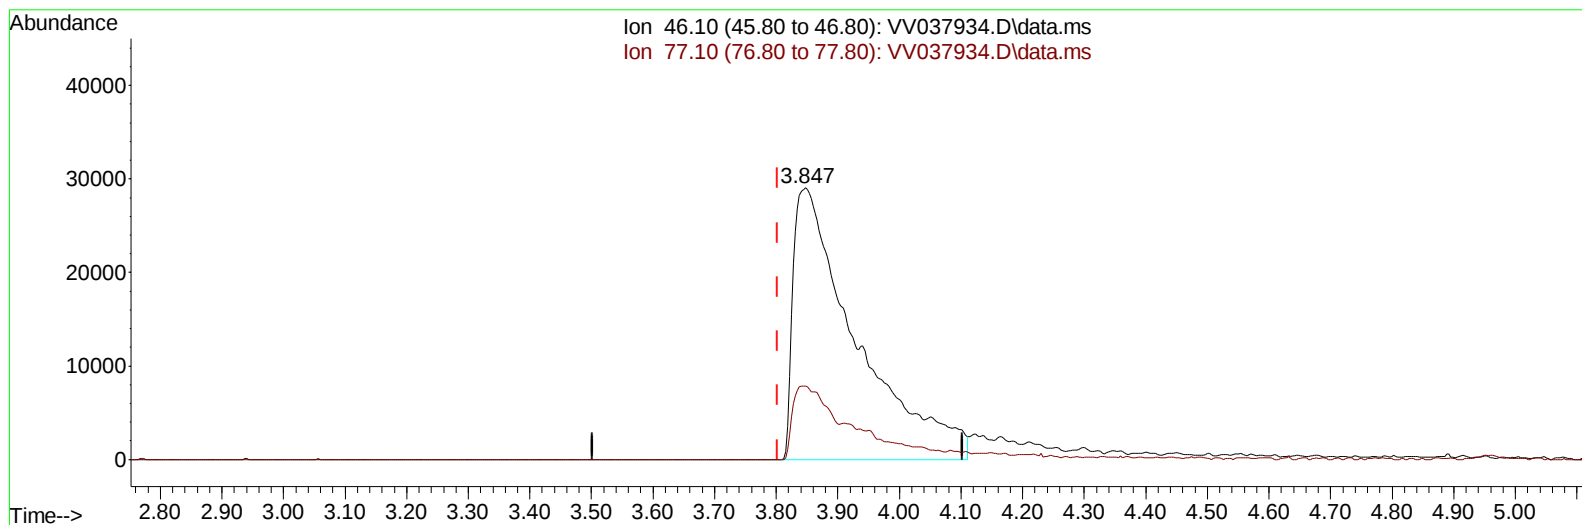

TIC: VV037934.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.045) 50.40 ug/L m

response 206266

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	26.30	15.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037934.D
 Acq On : 06 Nov 2024 17:34
 Operator : SY/MD
 Sample : P4714-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH9

Manual IntegrationsAPPROVED

Quant Time: Nov 06 22:47:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 06 22:44:19 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/07/2024
 Supervised By :Semsettin Yesilyurt 11/07/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		286891	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		301815	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152		137597	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		102379	4.662	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.200%	
7) Chloroethane-d5	1.529	69		77892	4.352	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	2.053	65		44687	4.689	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.800%	
20) 2-Butanone-d5	3.847	46		206266m	50.397	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.800%	
24) Chloroform-d	4.243	84		188466	4.708	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	4.944	65		90369	5.052	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%	
32) Benzene-d6	4.953	84		361803	4.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	5.985	67		113546	4.995	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.239	98		311336	4.451	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	7.561	79		40059	4.558	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%	
46) 2-Hexanone-d5	8.030	63		163977	48.010	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.020%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84		93391	5.096	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.000%	
66) 1,2-Dichlorobenzene-d4	11.558	152		121546	5.356	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037934.D
Acq On : 06 Nov 2024 17:34
Operator : SY/MD
Sample : P4714-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH9

Manual IntegrationsAPPROVED

Quant Time: Nov 06 22:47:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 22:44:19 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/07/2024
Supervised By :Semsettin Yesilyurt 11/07/2024

