

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037931.D
 Acq On : 06 Nov 2024 16:22
 Operator : SY/MD
 Sample : P4715-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Quant Time: Nov 06 22:46:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 06 22:44:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	270181	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	276531	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	130902	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	91071	4.404	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.000%
7) Chloroethane-d5	1.529	69	69556	4.127	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.600%
11) 1,1-Dichloroethene-d2	2.056	65	39893	4.445	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.000%
20) 2-Butanone-d5	3.815	46	160832	41.726	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.460%
24) Chloroform-d	4.246	84	162634	4.314	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
26) 1,2-Dichloroethane-d4	4.940	65	78477	4.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	4.953	84	312592	4.383	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	5.985	67	94207	4.524	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.400%
41) Toluene-d8	7.239	98	270665	4.223	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
43) trans-1,3-Dichloroprop...	7.561	79	32850	4.079	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	8.027	63	135330	43.246	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.500%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	78156	4.655	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%
66) 1,2-Dichlorobenzene-d4	11.557	152	105133	4.869	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds					Qvalue	
13) Acetone	2.137	43	29549	10.800	ug/L	99
16) Methylene chloride	2.442	84	451891	20.974	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037931.D
Acq On : 06 Nov 2024 16:22
Operator : SY/MD
Sample : P4715-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL0

Quant Time: Nov 06 22:46:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 22:44:19 2024
Response via : Initial Calibration

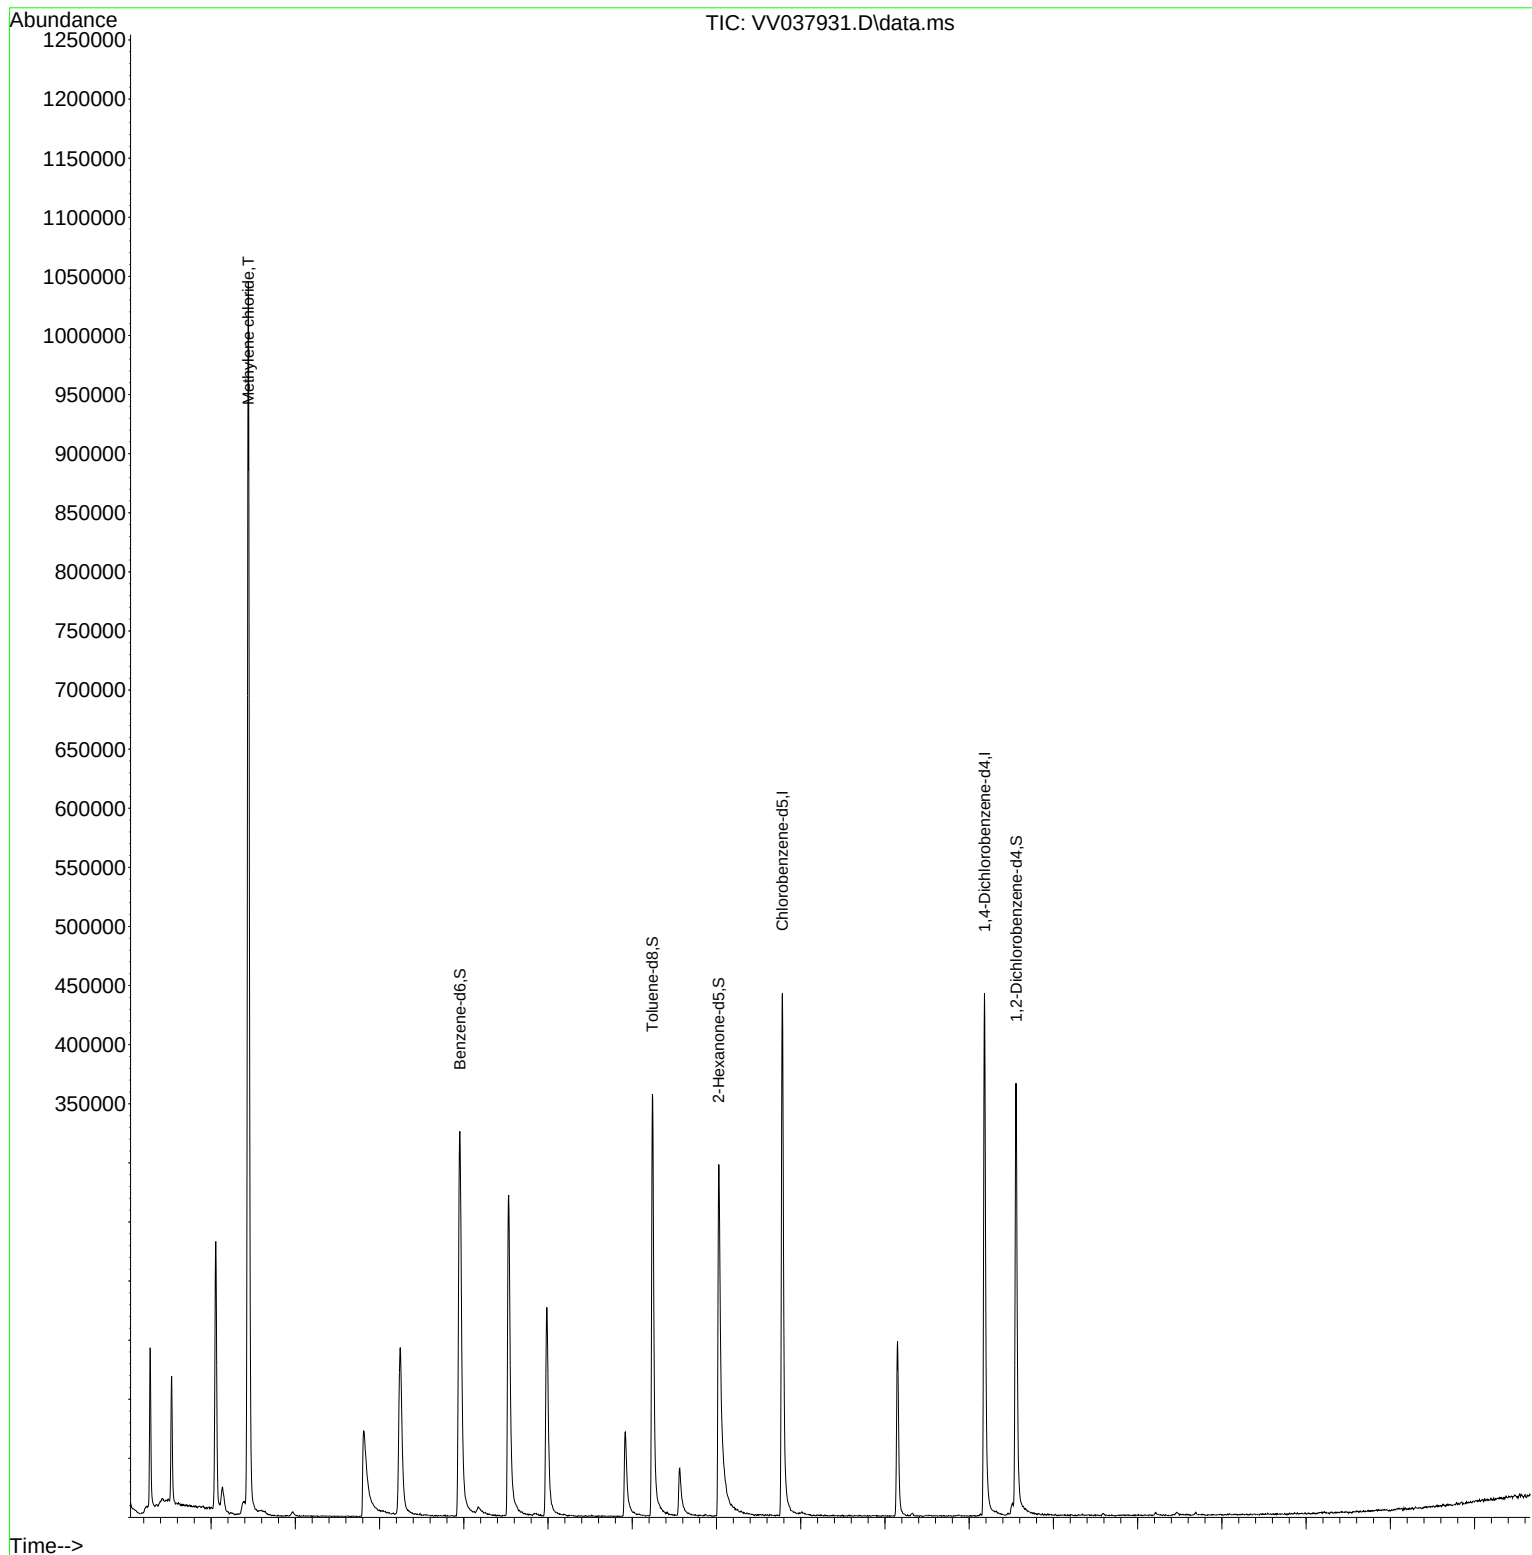

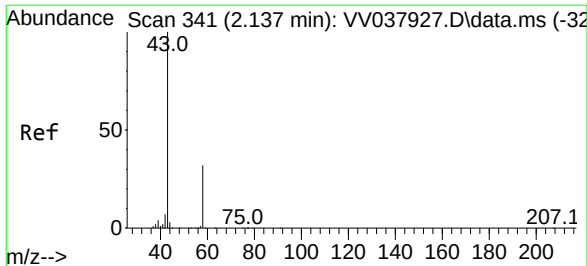

#13

Acetone

Concen: 10.800 ug/L

RT: 2.137 min Scan# 341

Delta R.T. -0.000 min

Lab File: VV037931.D

Acq: 06 Nov 2024 16:22

Instrument :

MSVOA_V

ClientSampleId :





COALO

Tgt Ion: 43 Resp: 29549

Ion Ratio Lower Upper

43 100

58 33.0 0.0 64.6

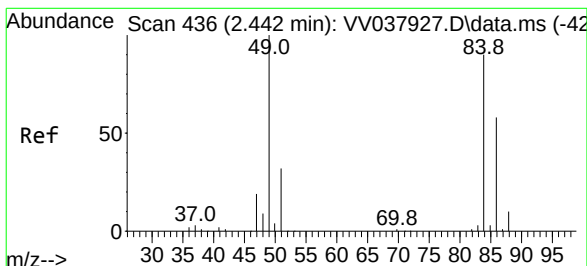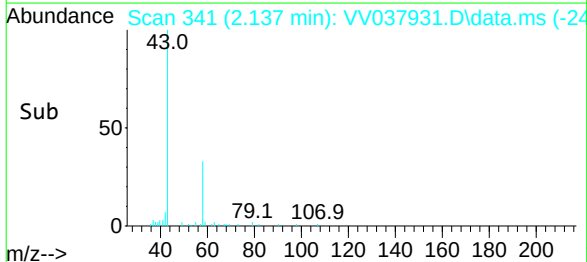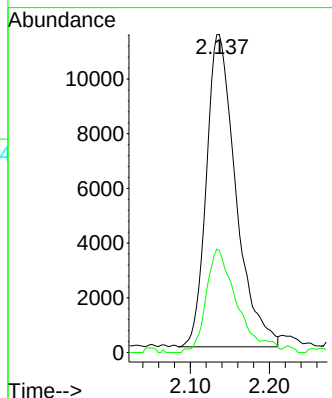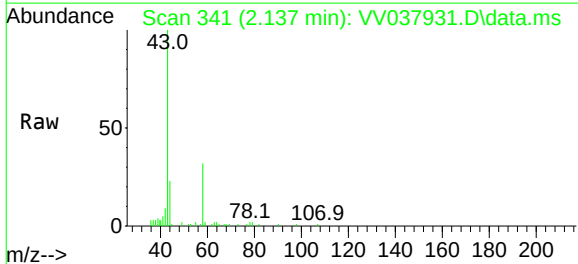

#16

Methylene chloride

Concen: 20.974 ug/L

RT: 2.442 min Scan# 436

Delta R.T. -0.000 min

Lab File: VV037931.D

Acq: 06 Nov 2024 16:22

Tgt Ion: 84 Resp: 451891

Ion Ratio Lower Upper

84 100

86 64.2 45.0 83.6

49 112.5 79.2 147.2

