

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037940.D
 Acq On : 06 Nov 2024 19:59
 Operator : SY/MD
 Sample : P4729-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B89

Quant Time: Nov 06 22:48:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 06 22:44:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	274400	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	287063	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	129604	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	101988	4.856	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.200%
7) Chloroethane-d5	1.529	69	81484	4.760	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.053	65	46117	5.060	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.200%
20) 2-Butanone-d5	3.831	46	198704	50.759	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.520%
24) Chloroform-d	4.243	84	190899	4.986	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	4.944	65	93167	5.445	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%
32) Benzene-d6	4.953	84	367352	4.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.986	67	111730	5.168	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.240	98	310445	4.666	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	7.561	79	36548	4.372	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.400%
46) 2-Hexanone-d5	8.027	63	162585	50.049	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.100%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	93302	5.353	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.000%
66) 1,2-Dichlorobenzene-d4	11.554	152	119182	5.575	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds					Qvalue	
34) Trichloroethene	5.838	95	11214	0.513	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037940.D
Acq On : 06 Nov 2024 19:59
Operator : SY/MD
Sample : P4729-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B89


Quant Time: Nov 06 22:48:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 06 22:44:19 2024
Response via : Initial Calibration

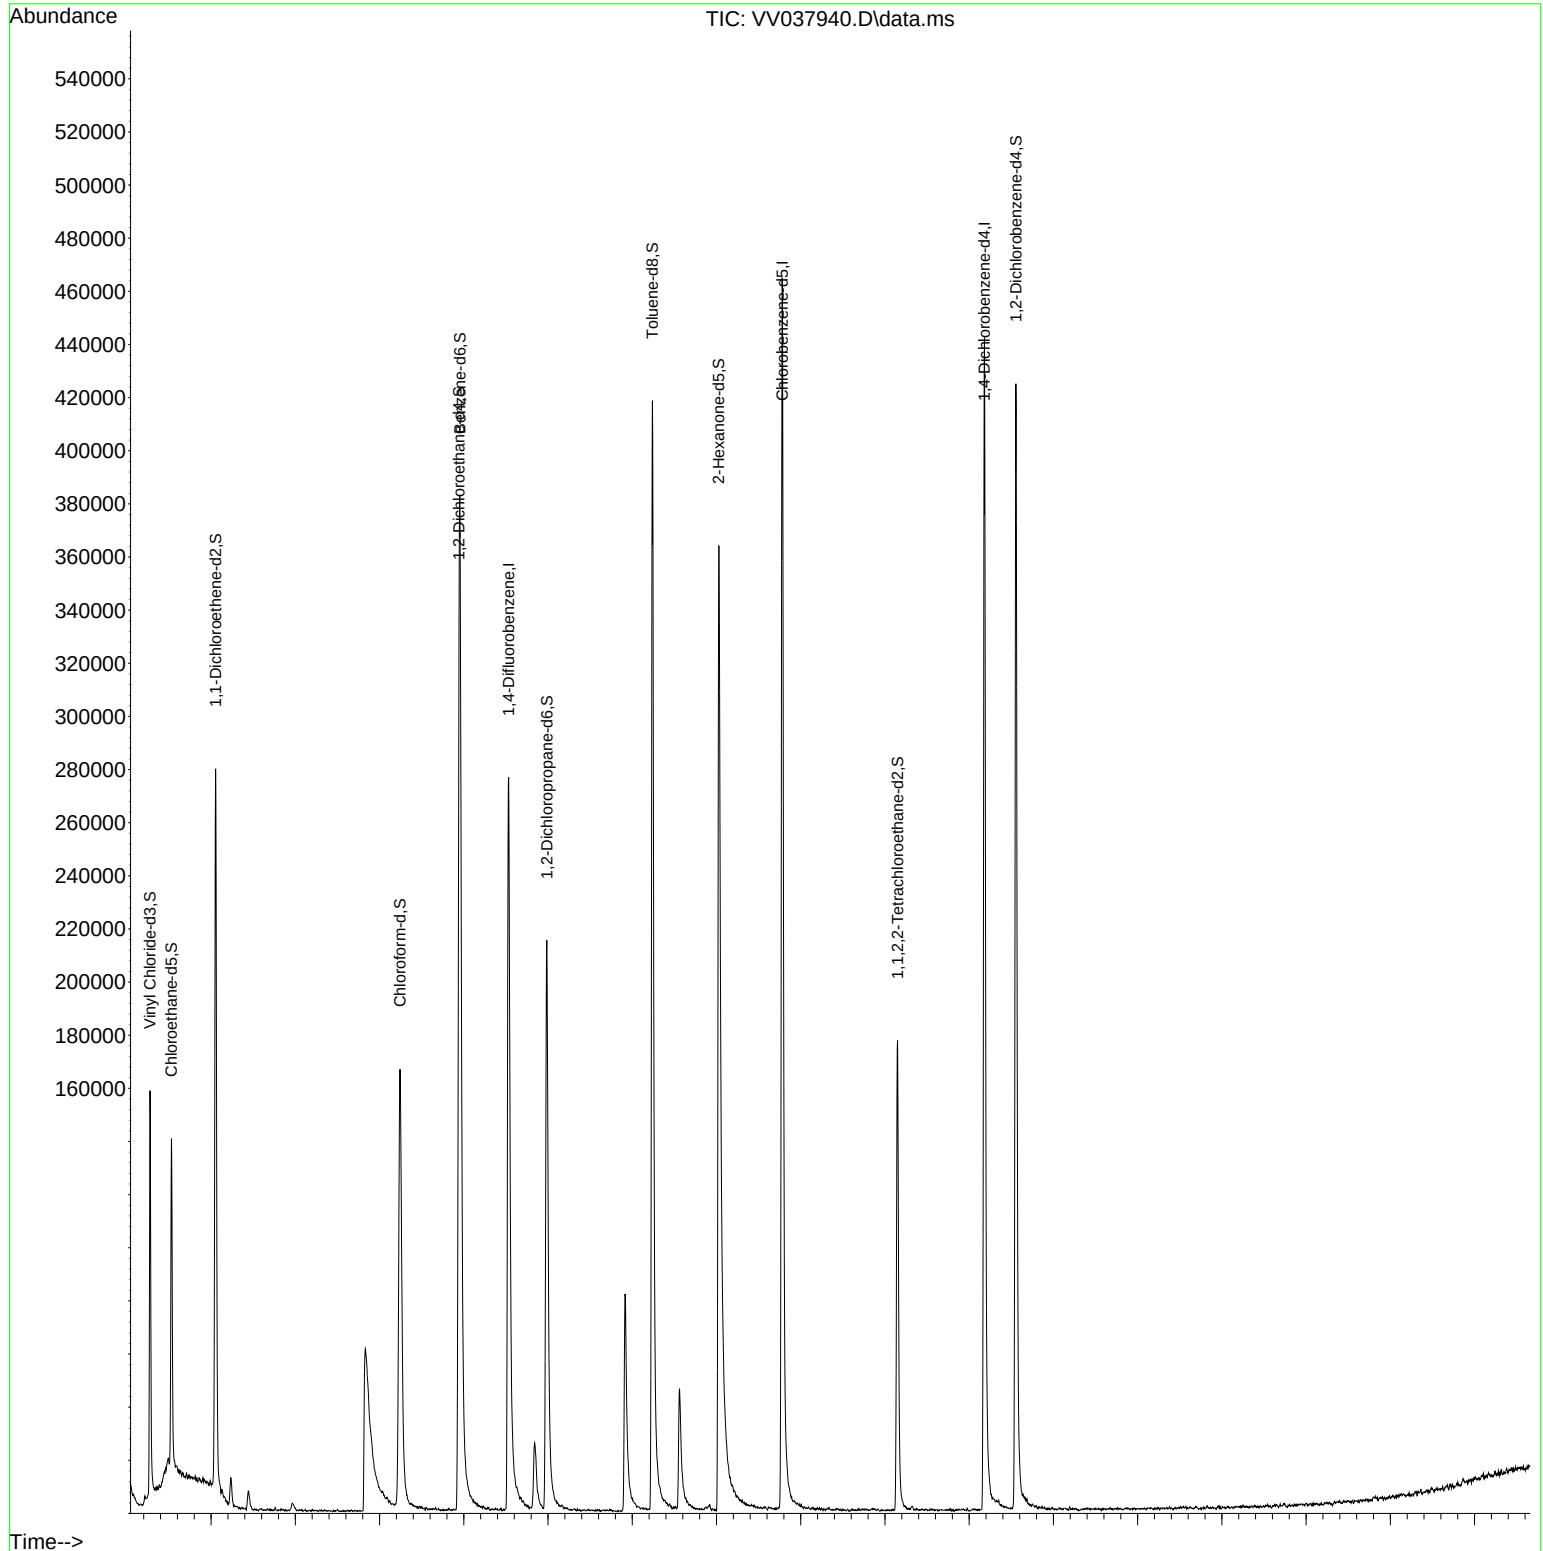

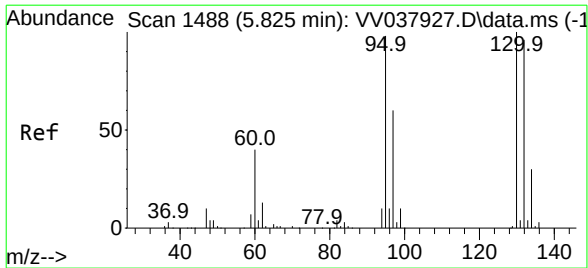

#34
 Trichloroethene
 Concen: 0.513 ug/L
 RT: 5.838 min Scan# 14
 Delta R.T. 0.013 min
 Lab File: VV037940.D
 Acq: 06 Nov 2024 19:59

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B89

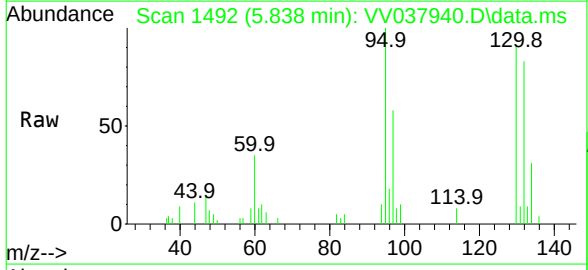

Tgt Ion:	95	Resp:	11214
Ion	Ratio	Lower	Upper
95	100		
97	58.3	46.9	87.1
132	83.0	70.5	130.9
130	91.1	72.9	135.3

