

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037928.D
 Acq On : 06 Nov 2024 15:06
 Operator : SY/MD
 Sample : VV1106WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV037928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	90	rBV	162291	178389	16.42%	1.946%
2	1.529	144	152	170	rVB	140629	165867	15.26%	1.810%
3	2.053	305	315	333	rBV	291406	420306	38.68%	4.585%
4	2.445	428	437	449	rBB3	6815	11072	1.02%	0.121%
5	3.834	854	869	919	rBV2	70501	392857	36.15%	4.286%
6	4.243	982	996	1027	rVB	173716	461339	42.46%	5.033%
7	4.950	1202	1216	1256	rBV2	415588	1086648	100.00%	11.855%
8	5.529	1387	1396	1429	rBV	311805	699394	64.36%	7.630%
9	5.985	1526	1538	1571	rBV	225311	510727	47.00%	5.572%
10	6.915	1816	1827	1861	rBV2	90224	211306	19.45%	2.305%
11	7.239	1917	1928	1970	rBV	468792	912355	83.96%	9.953%
12	7.558	2019	2027	2053	rBV2	50845	116338	10.71%	1.269%
13	8.027	2164	2173	2241	rBV	382183	1042289	95.92%	11.371%
14	8.780	2396	2407	2442	rBV	510192	919064	84.58%	10.026%
15	10.149	2821	2833	2860	rBV	177815	307025	28.25%	3.349%
16	11.181	3143	3154	3184	rBV	494949	861312	79.26%	9.396%
17	11.554	3256	3270	3298	rBV	466850	811649	74.69%	8.855%
18	13.210	3776	3785	3802	rBV10	7699	17469	1.61%	0.191%
19	13.451	3849	3860	3873	rBV2	9748	23696	2.18%	0.259%
20	13.683	3923	3932	3945	rBV8	8855	17285	1.59%	0.189%

Sum of corrected areas: 9166387




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037928.D
Acq On : 06 Nov 2024 15:06
Operator : SY/MD
Sample : VV1106WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

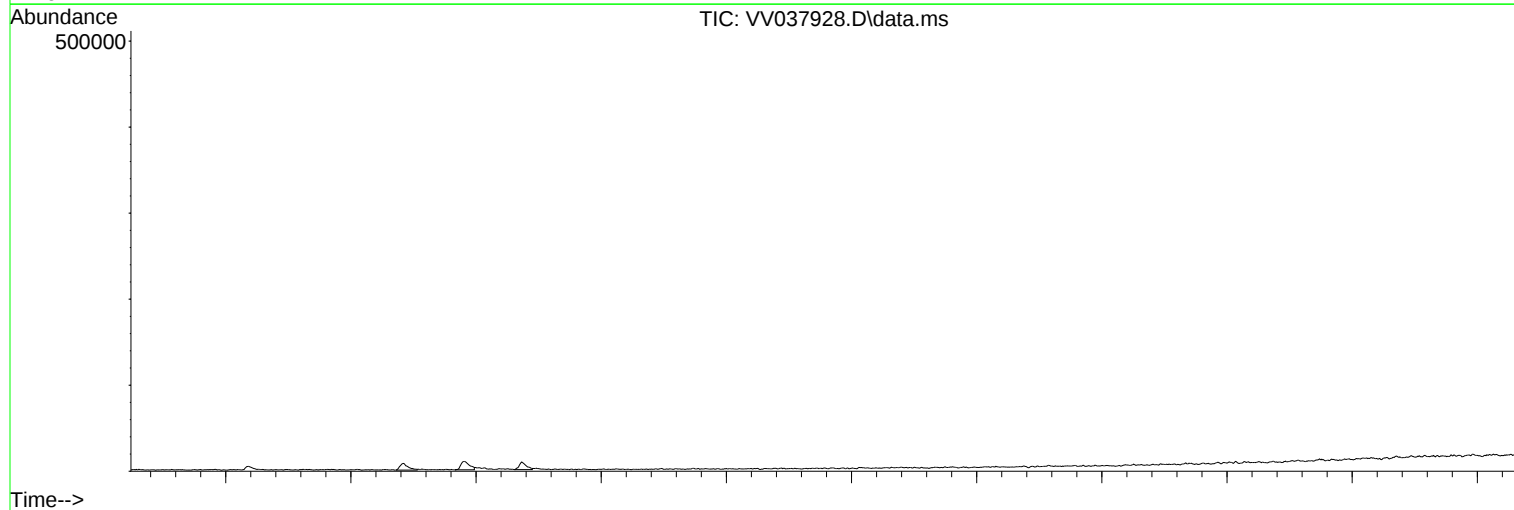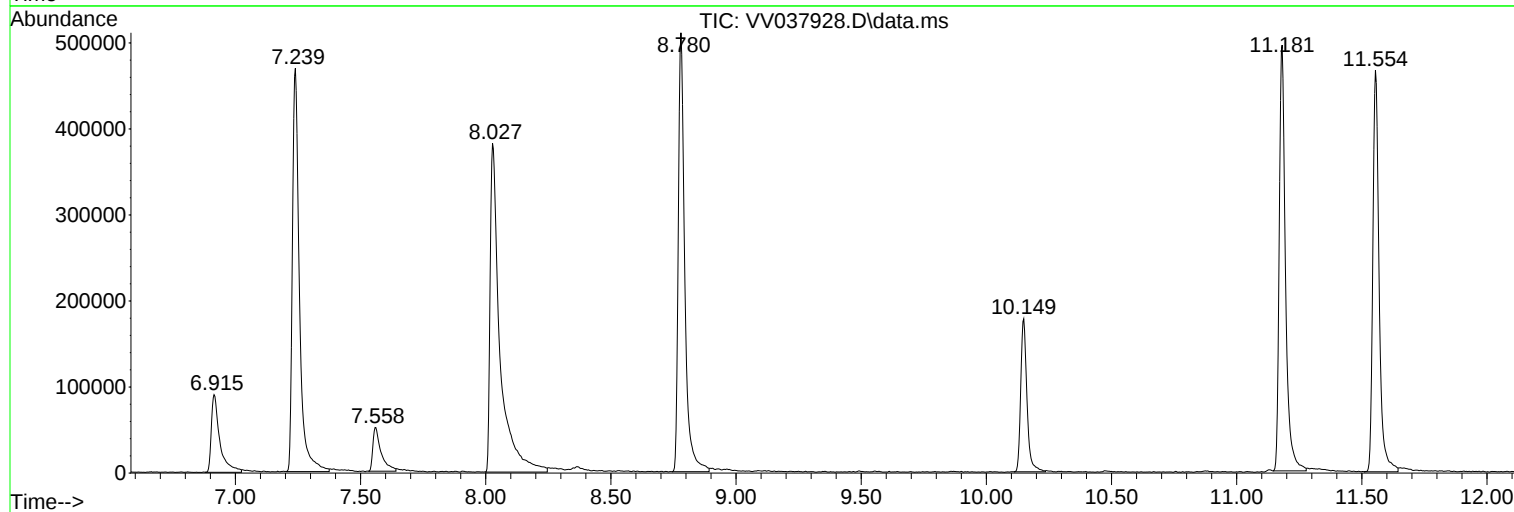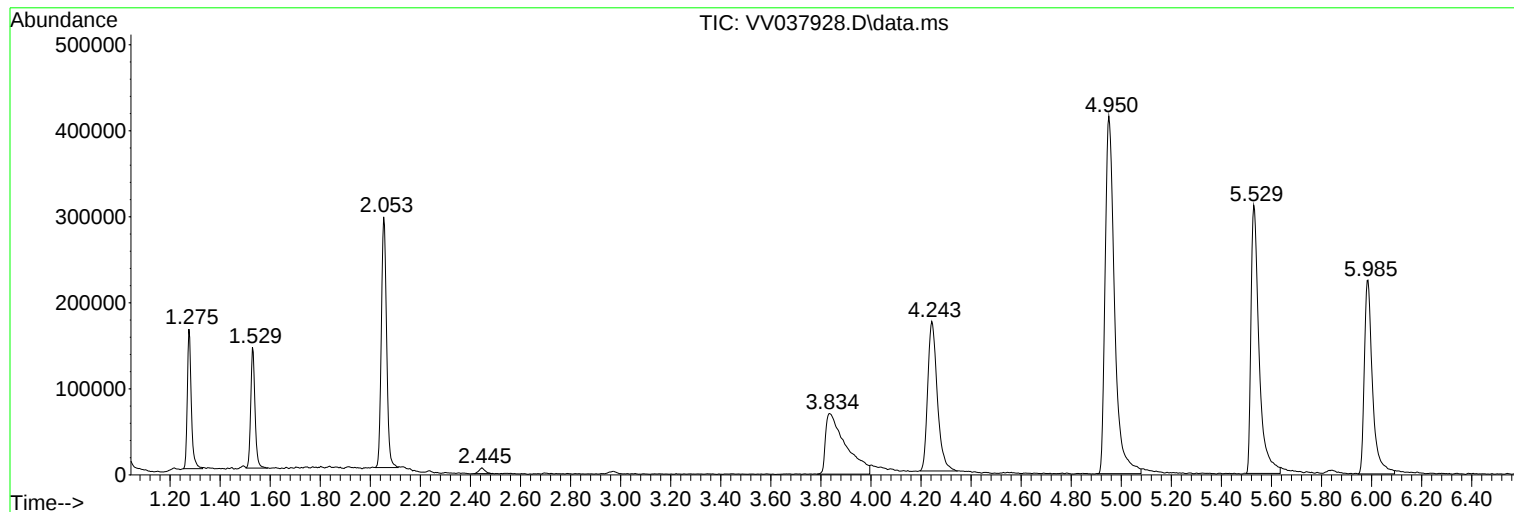

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037928.D
Acq On : 06 Nov 2024 15:06
Operator : SY/MD
Sample : VV1106WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037928.D
Acq On : 06 Nov 2024 15:06
Operator : SY/MD
Sample : VV1106WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc