

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037942.D
 Acq On : 06 Nov 2024 20:47
 Operator : SY/MD
 Sample : VIBLK392
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK392

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV037942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	65	73	89	rBV	173213	186414	16.48%	1.956%
2	1.529	145	152	163	rBV	139653	169033	14.94%	1.774%
3	2.053	305	315	328	rBV	291012	423163	37.40%	4.440%
4	2.442	427	436	447	rVB4	7292	12473	1.10%	0.131%
5	3.834	854	869	925	rBV3	74577	456210	40.32%	4.787%
6	4.243	980	996	1029	rBV	180991	482641	42.66%	5.064%
7	4.950	1201	1216	1247	rBV2	419142	1094451	96.74%	11.483%
8	5.532	1387	1397	1436	rBV	294963	676839	59.83%	7.101%
9	5.831	1478	1490	1521	rBV	136557	316283	27.96%	3.318%
10	5.986	1526	1538	1575	rVV	232406	521121	46.06%	5.468%
11	6.915	1815	1827	1855	rBV3	86318	199546	17.64%	2.094%
12	7.239	1915	1928	1963	rBV	456635	884309	78.16%	9.278%
13	7.561	2018	2028	2048	rBV2	49770	111852	9.89%	1.174%
14	7.908	2127	2136	2153	rVB5	10441	20551	1.82%	0.216%
15	8.027	2164	2173	2206	rBV2	454492	1131337	100.00%	11.870%
16	8.780	2396	2407	2439	rBV	506017	892222	78.86%	9.361%
17	10.149	2819	2833	2858	rBV	196745	345771	30.56%	3.628%
18	11.181	3143	3154	3178	rBV	463719	801314	70.83%	8.407%
19	11.554	3258	3270	3295	rBV	457842	789977	69.83%	8.289%
20	12.599	3591	3595	3604	rBV	18676	15442	1.36%	0.162%




Sum of corrected areas: 9530949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037942.D
Acq On : 06 Nov 2024 20:47
Operator : SY/MD
Sample : VIBLK392
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

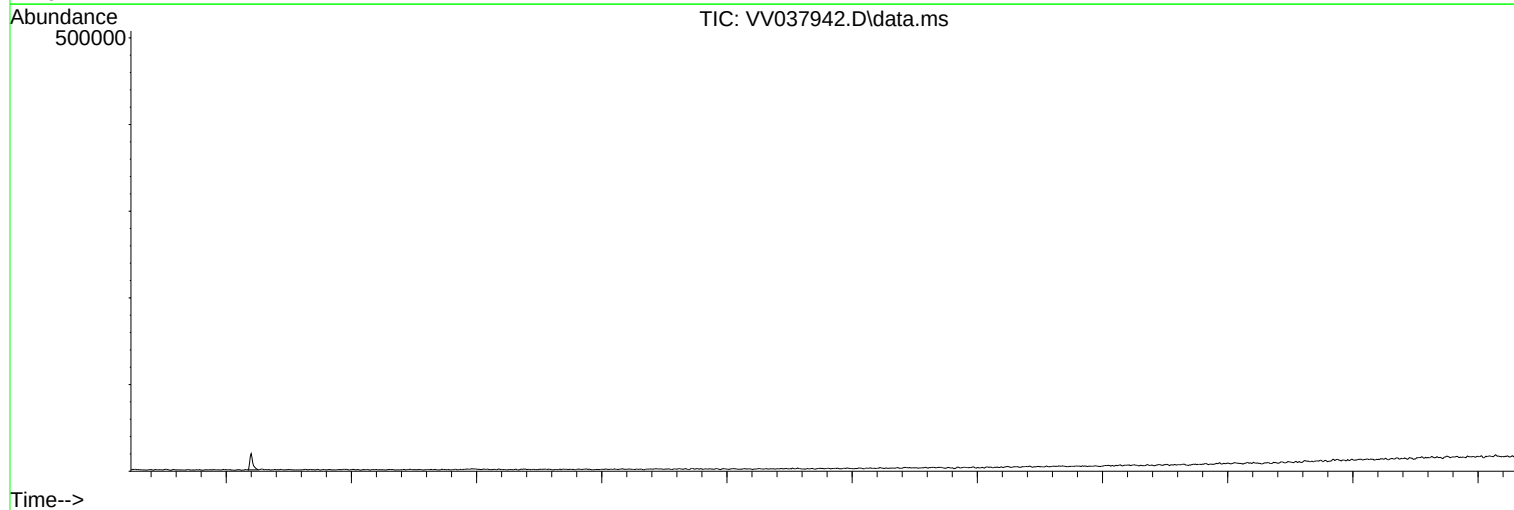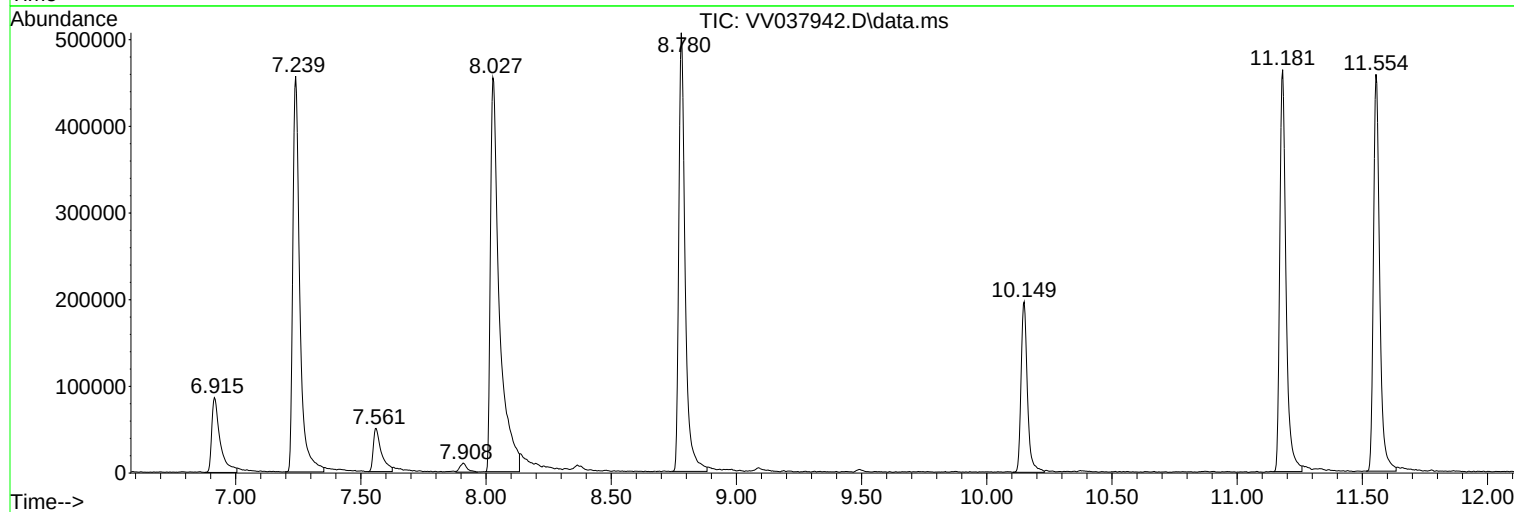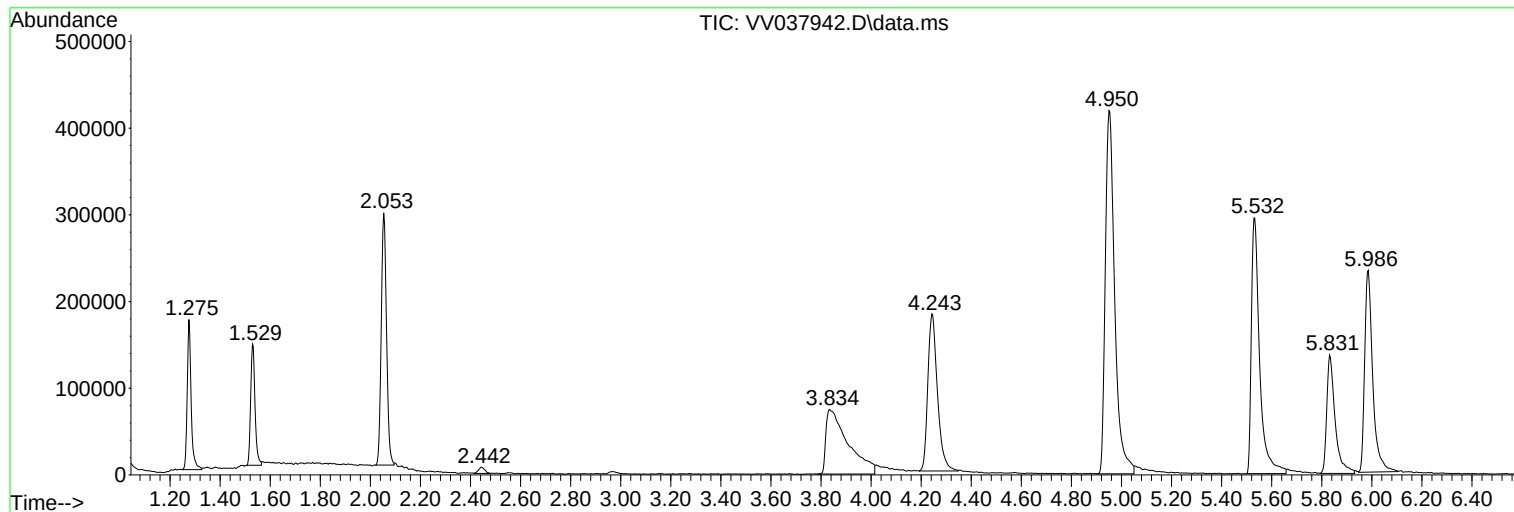

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037942.D
Acq On : 06 Nov 2024 20:47
Operator : SY/MD
Sample : VIBLK392
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
Data File : VV037942.D
Acq On : 06 Nov 2024 20:47
Operator : SY/MD
Sample : VIBLK392
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK392

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
