
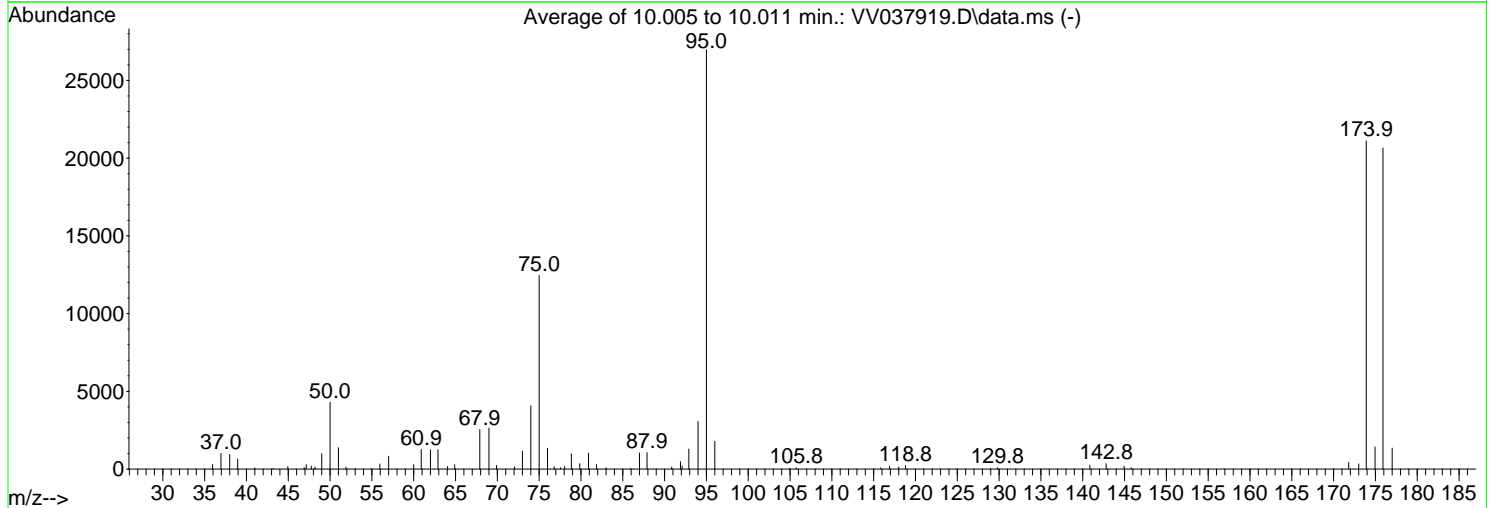


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110624\
 Data File : VV037919.D
 Acq On : 06 Nov 2024 09:14
 Operator : SY/MD
 Sample : BFB281
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB281

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 06 22:44:19 2024

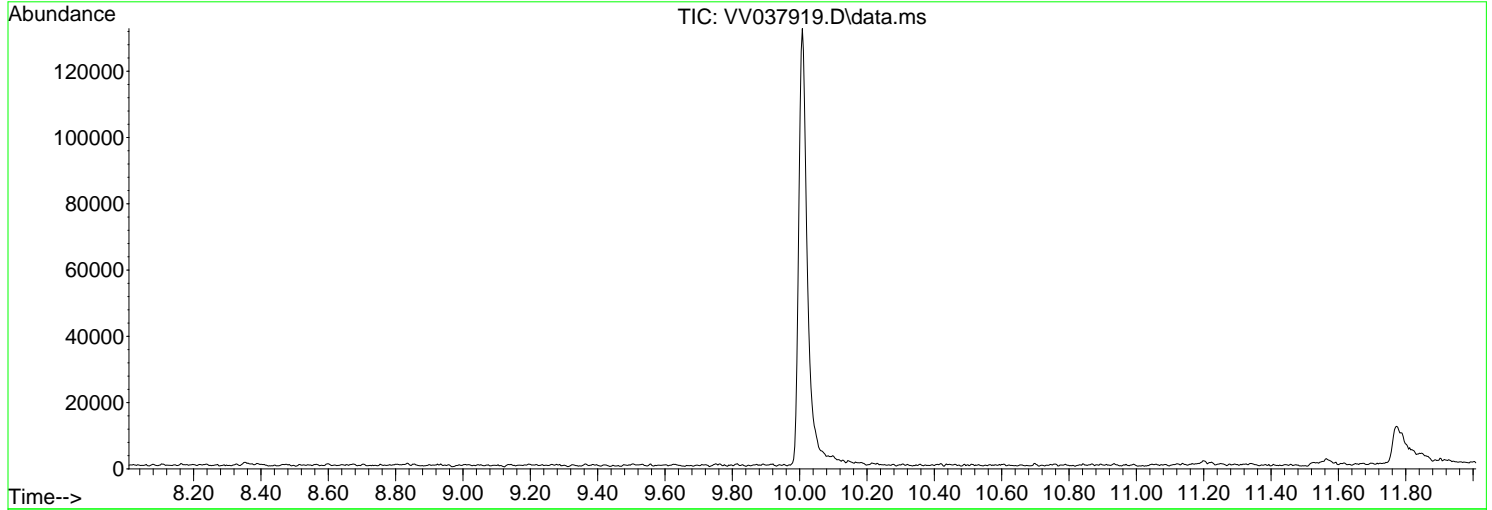

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	4301	PASS
75	95	30	80	46.2	12466	PASS
95	95	100	100	100.0	26973	PASS
96	95	5	9	6.6	1786	PASS
173	174	0.00	2	1.6	330	PASS
174	95	50	120	78.2	21104	PASS
175	174	5	9	6.7	1423	PASS
176	174	95	105	97.9	20653	PASS
177	176	5	10	6.5	1349	PASS

m/z	Abundance
35.90	321.0
36.90	1079.0
38.00	908.0
39.00	583.0
40.00	340.0
40.90	108.0
43.20	112.0
44.00	453.0
45.00	199.0
46.90	300.0
47.80	150.0
48.20	106.0
49.00	1067.0
50.00	4051.0
51.00	1471.0
51.90	142.0
55.00	118.0
56.00	290.0
57.00	767.0
60.00	283.0
60.90	1253.0
62.00	1163.0
62.90	1181.0
64.00	123.0
64.90	300.0
67.90	2542.0
69.00	2625.0
69.90	274.0
71.90	111.0
73.00	998.0
74.00	3801.0
75.00	11850.0
76.00	1213.0
76.80	317.0
78.00	205.0
78.90	1209.0
79.80	351.0
80.90	1026.0
81.90	307.0
83.00	111.0
87.00	1003.0
87.90	1018.0
90.80	117.0
92.10	616.0
92.90	1213.0
94.00	3175.0
95.00	25912.0
96.00	1616.0
105.80	126.0
116.90	170.0
118.00	114.0
118.80	216.0
129.80	130.0
140.80	251.0
142.80	374.0
144.90	203.0
145.80	157.0
171.80	385.0
173.00	316.0
173.90	21248.0
175.00	1439.0
175.90	21256.0
177.00	1330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	294.0
36.90	1025.0
38.00	966.0
39.00	676.0
40.00	327.0
44.00	464.0
45.00	148.0
47.00	282.0
47.20	283.0
47.80	213.0
48.20	148.0
49.00	1046.0
50.00	4388.0
51.00	1395.0
51.90	129.0
55.00	119.0
56.00	330.0
57.00	862.0
60.00	305.0
60.90	1289.0
62.00	1221.0
62.90	1320.0
64.00	172.0
64.90	276.0
67.90	2625.0
69.00	2734.0
69.90	234.0
72.10	141.0
73.00	1219.0
74.00	4220.0
75.00	12910.0
76.00	1389.0
76.80	305.0
77.50	105.0
78.00	184.0
78.90	1138.0
79.80	342.0
80.90	1043.0
81.80	301.0
83.00	127.0
87.00	1085.0
87.90	1072.0
90.90	136.0
91.90	690.0
92.90	1334.0
94.00	3230.0
95.00	27840.0
96.00	1878.0
105.70	119.0
115.90	108.0
116.90	169.0
118.00	148.0
118.80	252.0
129.00	103.0
129.80	133.0
140.90	257.0
142.80	323.0
145.00	194.0
145.80	114.0
171.80	436.0
173.00	357.0
173.90	21824.0
174.90	1443.0
175.90	21544.0
177.00	1370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	264.0
37.00	928.0
38.00	942.0
38.90	674.0
40.00	291.0
41.10	126.0
44.10	457.0
44.90	159.0
47.20	299.0
47.70	229.0
48.20	139.0
49.00	874.0
50.00	4463.0
51.00	1245.0
51.90	121.0
53.00	115.0
54.90	123.0
55.90	359.0
57.00	852.0
60.00	278.0
60.90	1240.0
62.00	1318.0
62.90	1231.0
64.10	203.0
64.90	274.0
67.90	2439.0
69.00	2570.0
69.90	210.0
72.10	175.0
73.00	1281.0
74.00	4183.0
75.00	12639.0
76.00	1408.0
76.80	254.0
77.60	164.0
78.10	150.0
78.90	908.0
79.90	352.0
80.90	1021.0
81.80	296.0
85.90	108.0
87.00	1022.0
87.90	1091.0
90.90	142.0
91.90	738.0
92.90	1325.0
94.00	2782.0
95.00	27168.0
96.00	1863.0
104.90	113.0
115.80	138.0
116.90	168.0
118.00	141.0
118.80	248.0
140.90	254.0
142.80	321.0
145.00	166.0
171.80	450.0
173.00	316.0
173.90	20240.0
174.90	1387.0
175.90	19160.0
177.00	1347.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
39.90	337.0
44.00	553.0
54.80	116.0
76.90	133.0
78.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281