


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110718\
Data File : VV008542.D
Acq On : 07 Nov 2018 10:19
Operator : SY/MD
Sample : BFB42
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR110718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 07 14:54:38 2018

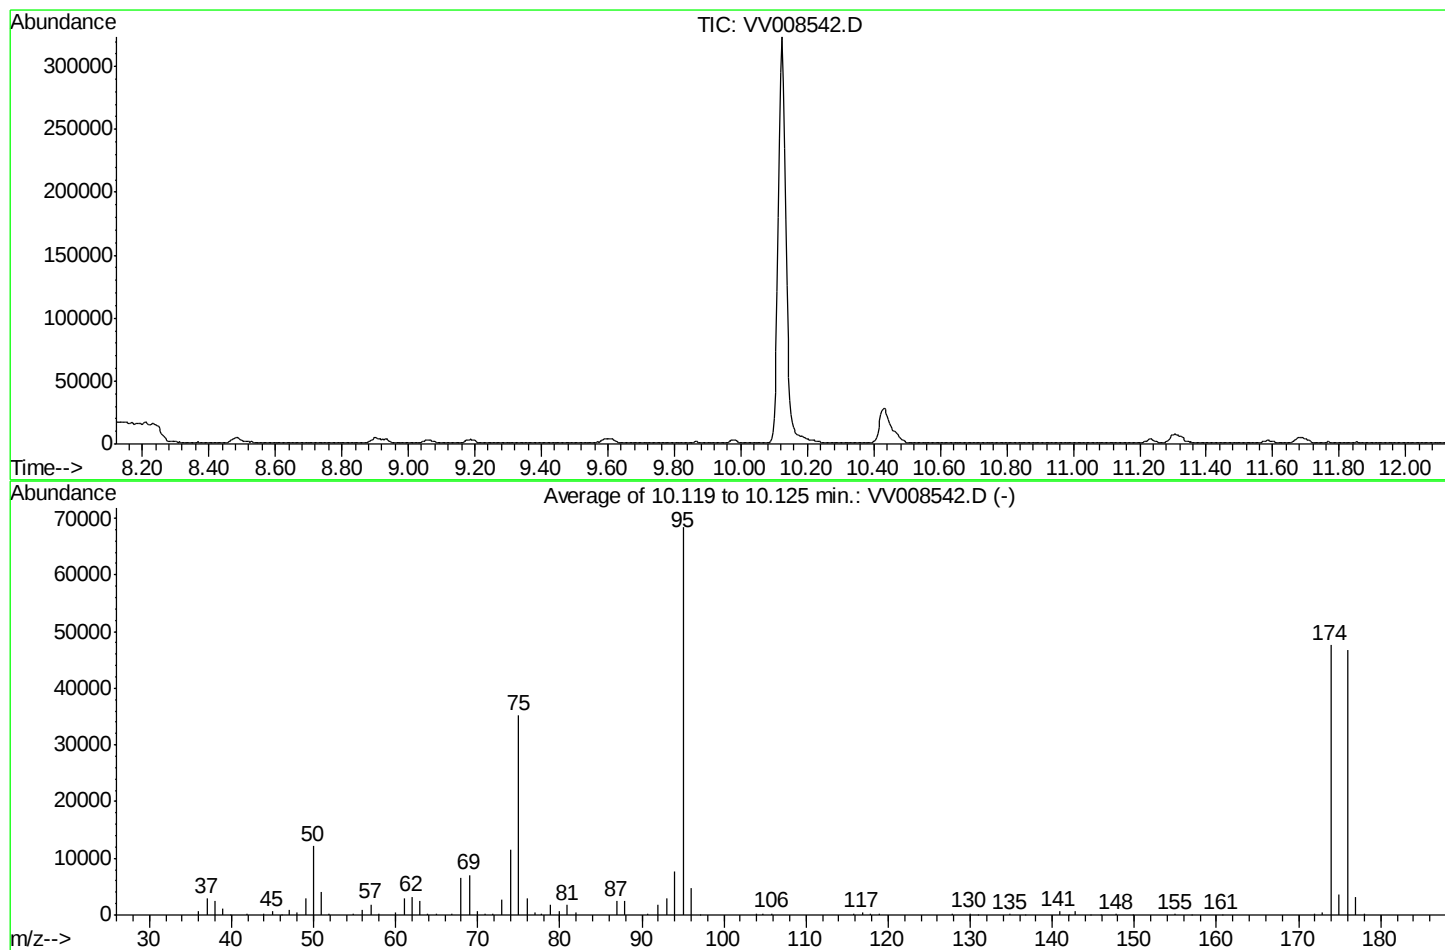

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12096	PASS
75	95	30	80	51.5	35208	PASS
95	95	100	100	100.0	68389	PASS
96	95	5	9	6.8	4644	PASS
173	174	0.00	2	1.2	549	PASS
174	95	50	120	69.5	47554	PASS
175	174	5	9	7.6	3608	PASS
176	174	95	101	98.2	46701	PASS
177	176	5	9	6.7	3145	PASS

Scan 2796 (10.080 min): VV008542.D
BFB42

m/z	Abundance
39.90	198.0
43.00	121.0
43.90	539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	639.0
37.00	2890.0
38.00	2372.0
39.00	1160.0
39.90	201.0
41.90	130.0
44.00	803.0
45.00	562.0
47.00	919.0
48.00	450.0
49.00	2595.0
50.00	11542.0
51.00	3810.0
51.90	161.0
54.90	181.0
56.00	930.0
57.00	1906.0
57.90	127.0
60.00	512.0
61.00	3008.0
62.00	3240.0
63.00	2308.0
63.90	215.0
64.90	186.0
66.80	160.0
68.00	6279.0
69.00	6892.0
70.00	668.0
70.90	108.0
71.80	306.0
73.00	2690.0
74.00	10683.0
75.00	33544.0
76.00	2819.0
77.00	427.0
77.80	249.0
78.90	1786.0
80.00	515.0
80.90	1714.0
81.90	504.0
87.00	2257.0
88.00	2339.0
90.70	249.0
92.00	1637.0
93.00	2734.0
94.00	7366.0
95.00	64888.0
96.00	4602.0
103.90	297.0
104.80	135.0
105.90	338.0
115.80	215.0
116.90	316.0
117.80	181.0
118.90	354.0
127.90	156.0
129.90	243.0
130.90	142.0
134.90	132.0
140.90	585.0
142.80	531.0
145.90	118.0
147.80	138.0
149.80	107.0
154.90	155.0
172.10	299.0
172.90	443.0
173.90	44240.0
174.90	3405.0
175.90	43344.0
176.90	2953.0
178.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	709.0
37.00	3026.0
38.00	2576.0
39.00	1257.0
39.90	223.0
41.90	137.0
42.90	123.0
43.90	833.0
44.90	661.0
47.00	873.0
47.90	468.0
49.00	2985.0
50.00	12460.0
51.00	4135.0
51.90	195.0
54.90	208.0
56.00	1039.0
57.00	1935.0
57.90	134.0
60.00	540.0
61.00	3049.0
62.00	3281.0
63.00	2545.0
63.90	254.0
65.00	185.0
66.90	168.0
68.00	6826.0
69.00	7270.0
70.00	628.0
70.90	130.0
71.90	304.0
73.00	2912.0
74.00	11857.0
75.00	36496.0
76.00	3077.0
77.00	421.0
77.80	301.0
78.90	1970.0
79.90	582.0
80.90	1793.0
81.90	505.0
87.00	2575.0
87.90	2496.0
90.80	268.0
92.00	1915.0
93.00	3131.0
94.00	7903.0
95.00	70704.0
96.00	4763.0
97.00	121.0
103.90	298.0
104.80	142.0
105.90	356.0
115.90	255.0
116.80	364.0
117.80	247.0
118.90	346.0
127.90	203.0
129.90	246.0
130.90	131.0
134.90	164.0
136.70	105.0
140.90	615.0
141.90	140.0
142.90	608.0
144.70	116.0
145.80	119.0
147.80	131.0
149.80	105.0
154.90	174.0
156.90	126.0
172.00	273.0
172.90	577.0
173.90	49144.0
175.00	3705.0
176.00	48400.0
177.00	3322.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	649.0
37.00	2850.0
38.00	2559.0
39.00	1325.0
39.90	241.0
42.00	122.0
42.90	154.0
43.90	828.0
44.90	657.0
46.10	111.0
47.00	755.0
47.90	451.0
49.00	2953.0
50.00	12288.0
51.00	3994.0
52.00	214.0
54.90	192.0
56.00	1004.0
57.00	1720.0
57.90	122.0
60.00	523.0
61.00	2938.0
62.00	3238.0
63.00	2582.0
63.90	286.0
65.00	174.0
66.90	206.0
68.00	6779.0
69.00	7101.0
70.00	560.0
70.90	127.0
71.90	301.0
73.00	2885.0
74.00	12006.0
75.00	35584.0
76.00	3014.0
77.00	364.0
77.80	317.0
78.90	1978.0
79.90	619.0
80.90	1776.0
81.90	491.0
86.90	2599.0
87.90	2546.0
90.80	271.0
92.00	2017.0
93.00	3272.0
94.00	7931.0
95.00	69576.0
96.00	4567.0
97.10	118.0
103.90	284.0
104.80	143.0
105.90	302.0
115.90	277.0
116.80	404.0
117.80	275.0
118.90	311.0
127.80	246.0
130.00	222.0
134.90	149.0
136.70	116.0
140.90	582.0
142.00	173.0
142.90	631.0
144.70	115.0
145.80	112.0
147.80	117.0
155.00	148.0
156.90	134.0
160.70	112.0
171.90	276.0
172.90	629.0
173.90	49280.0
175.00	3714.0
176.00	48360.0
176.90	3162.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42