

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019272.D
 Acq On : 05 Nov 2020 12:27
 Operator : SY/MD
 Sample : L4615-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG465

Quant Time: Nov 05 23:11:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 05 22:32:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	221211	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	217160	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	109616	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	91200	51.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.76%
7) Chloroethane-d5	1.58	69	74687	54.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.38%
11) 1,1-Dichloroethene-d2	2.12	63	139720	41.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.56%
21) 2-Butanone-d5	3.90	46	112430	104.42	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.42%
24) Chloroform-d	4.37	84	170541	52.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.30%
26) 1,2-Dichloroethane-d4	5.05	65	120308	52.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.60%
32) Benzene-d6	5.07	84	324120	52.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.22%
36) 1,2-Dichloropropane-d6	6.09	67	101169	55.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.16%
41) Toluene-d8	7.33	98	296046	50.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.06%
43) trans-1,3-Dichloropropene-	7.64	79	53230	50.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.16%
47) 2-Hexanone-d5	8.10	63	74449	93.59	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.59%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	122112	49.31	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.62%
64) 1,2-Dichlorobenzene-d4	11.65	152	125899	54.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.34%


Target Compounds					Ovalue
13) Acetone	2.18	43	5343	5.341 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110720\
Data File : VV019272.D
Acq On : 05 Nov 2020 12:27
Operator : SY/MD
Sample : L4615-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG465

Quant Time: Nov 05 23:11:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 05 22:32:19 2020
Response via : Initial Calibration

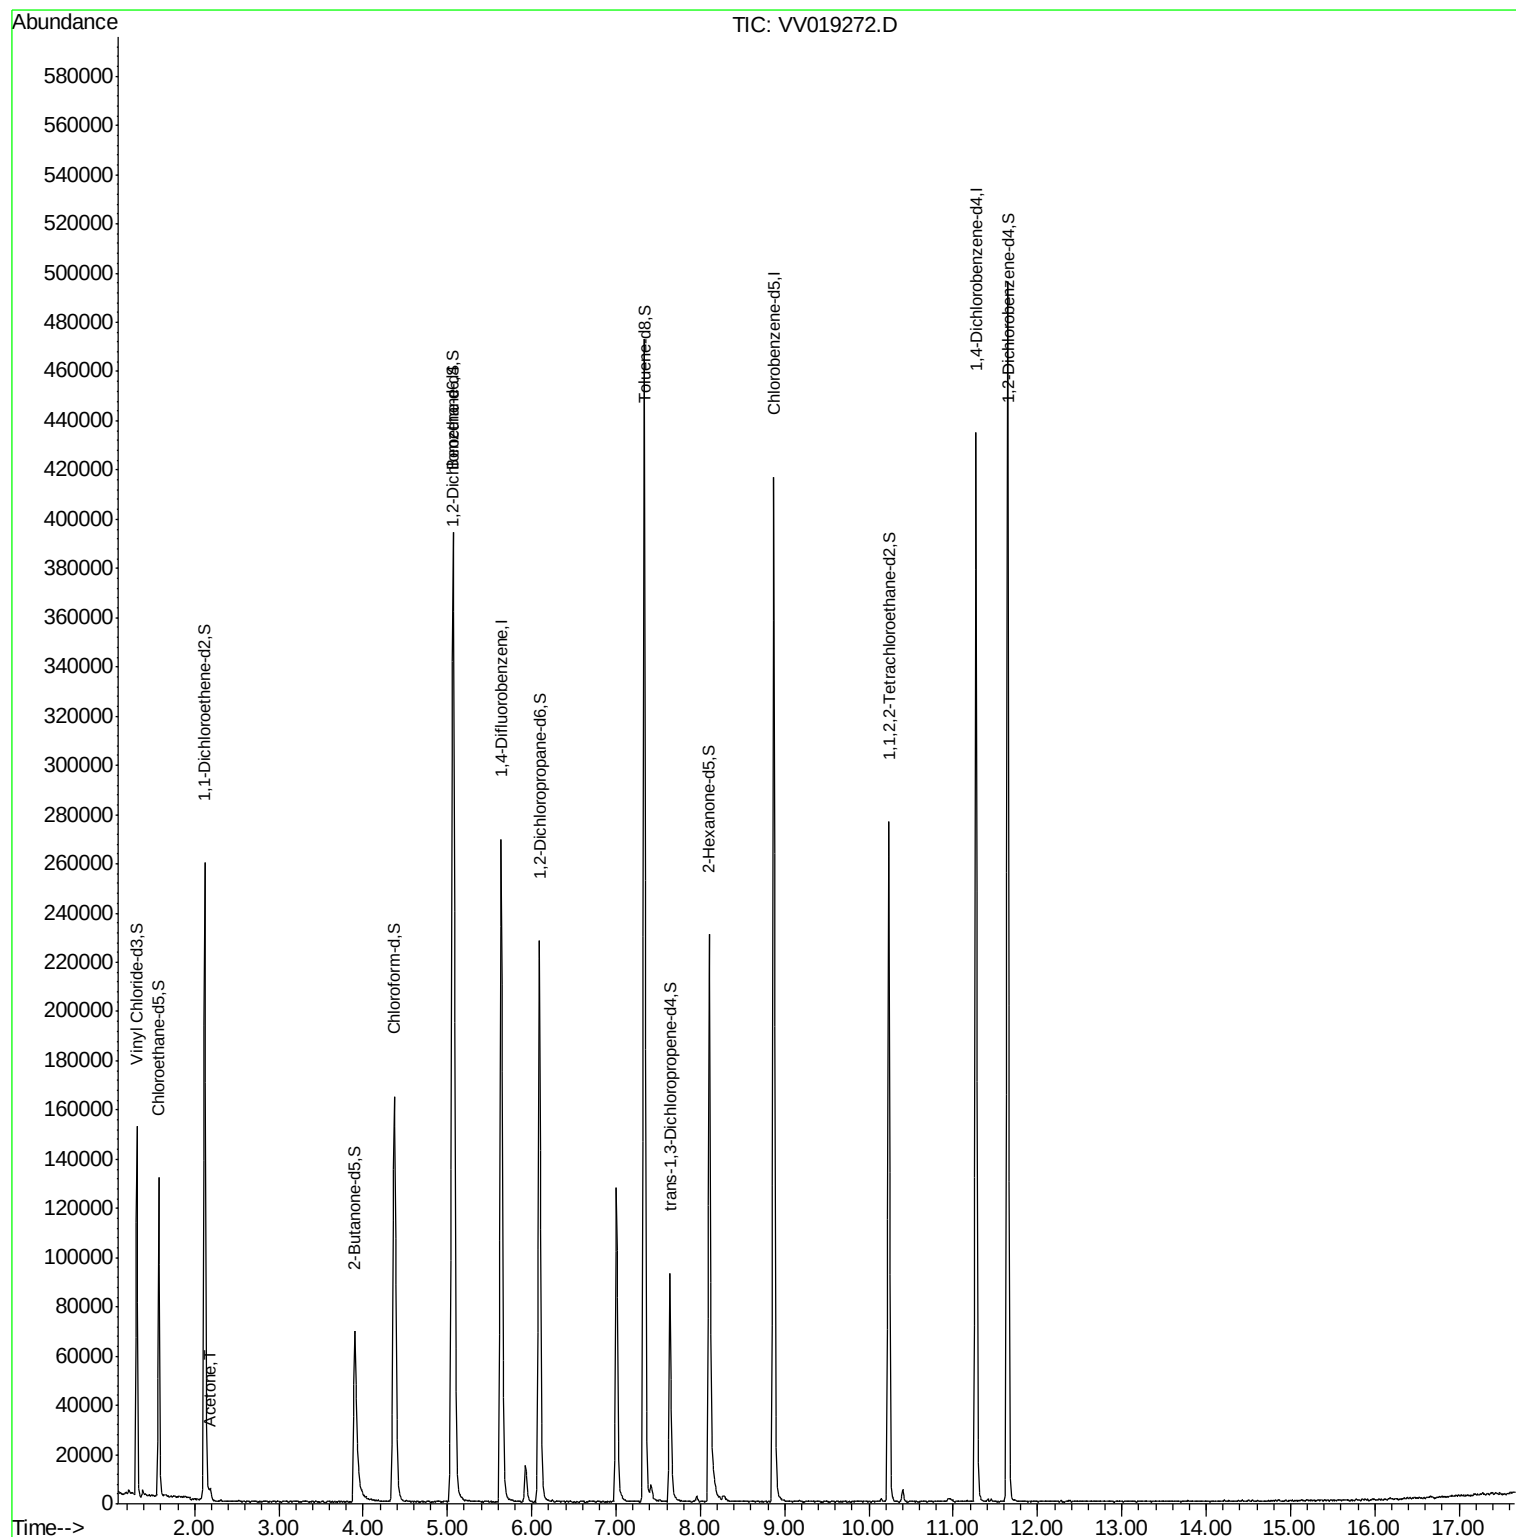

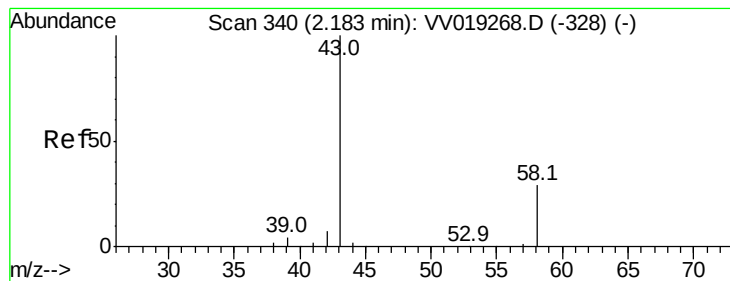

#13
Acetone
Concen: 5.341 ug/L
RT: 2.18 min Scan# 340
Delta R.T. 0.00 min
Lab File: VV019272.D
Acq: 05 Nov 2020 12:27

Instrument :
MSVOA_V
ClientSampleId :
BG465

Tot Ion: 43 Resp: 5343
Ion Ratio Lower Upper
43 100
58 29.8 0.0 59.4

