

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019271.D
 Acq On : 05 Nov 2020 11:51
 Operator : SY/MD
 Sample : L4543-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC: VV0192271.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	152832	153186	14.85%	1.971%
2	1.579	144	152	163	rBV	134650	151302	14.67%	1.946%
3	2.123	310	321	341	rVB	259626	387277	37.54%	4.982%
4	2.495	433	437	441	rBV	249	276	0.03%	0.004%
5	2.708	502	503	508	rVB2	271	171	0.02%	0.002%
6	2.737	509	512	513	rBV	169	90	0.01%	0.001%
7	2.856	545	549	556	rBV2	375	520	0.05%	0.007%
8	2.894	558	561	564	rVV	146	77	0.01%	0.001%
9	3.023	600	601	604	rVB	231	84	0.01%	0.001%
10	3.071	612	616	620	rBV2	218	238	0.02%	0.003%
11	3.103	622	626	632	rVV2	210	276	0.03%	0.004%
12	3.196	652	655	657	rBV2	248	151	0.01%	0.002%
13	3.319	691	693	696	rBV	209	101	0.01%	0.001%
14	3.444	730	732	737	rBV2	213	157	0.02%	0.002%
15	3.508	748	752	756	rBV	298	274	0.03%	0.004%
16	3.595	777	779	780	rBV	104	39	0.00%	0.001%
17	3.672	801	803	806	rBV2	127	64	0.01%	0.001%
18	3.692	806	809	812	rBV2	277	247	0.02%	0.003%
19	3.708	812	814	817	rBV	132	78	0.01%	0.001%
20	3.759	827	830	831	rBV	194	108	0.01%	0.001%
21	3.830	850	852	854	rVB	155	63	0.01%	0.001%
22	3.868	858	864	865	rBV	235	245	0.02%	0.003%
23	3.907	865	876	914	rBV2	74626	214689	20.81%	2.762%
24	4.376	1005	1022	1045	rBV	169444	416887	40.41%	5.363%
25	4.550	1073	1076	1077	rBV	189	89	0.01%	0.001%
26	4.621	1095	1098	1101	rBV2	285	208	0.02%	0.003%
27	4.679	1113	1116	1119	rBV2	324	186	0.02%	0.002%
28	4.762	1139	1142	1145	rBV2	233	183	0.02%	0.002%
29	4.798	1151	1153	1158	rVB2	234	176	0.02%	0.002%
30	4.888	1174	1181	1186	rBV2	346	458	0.04%	0.006%
31	4.968	1203	1206	1210	rBV2	437	403	0.04%	0.005%
32	5.071	1219	1238	1264	rBV2	401271	1031679	100.00%	13.272%
33	5.386	1332	1336	1338	rBV3	368	283	0.03%	0.004%
34	5.560	1387	1390	1392	rBV2	316	167	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019271.D
 Acq On : 05 Nov 2020 11:51
 Operator : SY/MD
 Sample : L4543-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1443	rBV	288585	572713	55.51%	7.367%
36	5.855	1479	1482	1484	rBV	369	286	0.03%	0.004%
37	5.929	1495	1505	1523	rBV3	14615	30309	2.94%	0.390%
38	6.093	1543	1556	1582	rBV	230498	465840	45.15%	5.993%
39	6.399	1649	1651	1653	rBV	194	60	0.01%	0.001%
40	6.431	1656	1661	1663	rBV2	186	210	0.02%	0.003%
41	6.482	1673	1677	1679	rBV	197	180	0.02%	0.002%
42	6.527	1689	1691	1693	rBV2	145	78	0.01%	0.001%
43	6.669	1732	1735	1736	rBV	363	186	0.02%	0.002%
44	6.846	1784	1790	1793	rBV	268	278	0.03%	0.004%
45	6.962	1822	1826	1828	rBV	261	199	0.02%	0.003%
46	7.007	1830	1840	1865	rVV	134002	240229	23.29%	3.090%
47	7.338	1931	1943	1961	rBV	471648	811398	78.65%	10.438%
48	7.598	2021	2024	2026	rBV	372	270	0.03%	0.003%
49	7.643	2028	2038	2061	rVV	95709	166055	16.10%	2.136%
50	8.013	2152	2153	2158	rVB2	258	160	0.02%	0.002%
51	8.106	2172	2182	2222	rBV	252372	461632	44.75%	5.939%
52	8.370	2262	2264	2266	rBV	447	303	0.03%	0.004%
53	8.511	2304	2308	2311	rBV3	383	317	0.03%	0.004%
54	8.637	2343	2347	2349	rBV2	411	377	0.04%	0.005%
55	8.823	2403	2405	2409	rVB	243	110	0.01%	0.001%
56	8.871	2409	2420	2442	rBV	442335	723045	70.08%	9.301%
57	9.090	2487	2488	2491	rVB2	346	140	0.01%	0.002%
58	9.222	2526	2529	2535	rBV2	310	409	0.04%	0.005%
59	9.373	2572	2576	2577	rBV	225	159	0.02%	0.002%
60	9.788	2703	2705	2709	rBV2	218	185	0.02%	0.002%
61	10.039	2781	2783	2785	rBV2	184	100	0.01%	0.001%
62	10.074	2791	2794	2798	rVB	221	150	0.01%	0.002%
63	10.096	2798	2801	2802	rBV	210	115	0.01%	0.001%
64	10.238	2830	2845	2868	rBV	280231	449385	43.56%	5.781%
65	10.338	2874	2876	2880	rBV2	349	311	0.03%	0.004%
66	10.460	2911	2914	2915	rBV	189	97	0.01%	0.001%
67	10.608	2954	2960	2963	rBV3	481	623	0.06%	0.008%
68	10.794	3015	3018	3023	rVB2	257	218	0.02%	0.003%
69	10.826	3023	3028	3031	rBV2	493	584	0.06%	0.008%
70	10.897	3047	3050	3055	rBV	312	328	0.03%	0.004%
71	10.939	3057	3063	3071	rVV4	1294	1908	0.18%	0.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110720\
 Data File : VV019271.D
 Acq On : 05 Nov 2020 11:51
 Operator : SY/MD
 Sample : L4543-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	11.055	3096	3099	3102	rBV2	180	156	0.02%	0.002%
73	11.196	3139	3143	3146	rBV2	318	284	0.03%	0.004%
74	11.270	3155	3166	3184	rBV	448775	696839	67.54%	8.964%
75	11.646	3270	3283	3303	rBV	493181	783894	75.98%	10.084%
76	11.823	3335	3338	3341	rBV	442	348	0.03%	0.004%
77	11.849	3344	3346	3353	rVB	241	200	0.02%	0.003%
78	12.141	3433	3437	3440	rBV2	285	256	0.02%	0.003%
79	12.251	3466	3471	3474	rBV	309	319	0.03%	0.004%
80	12.665	3595	3600	3603	rBV2	289	348	0.03%	0.004%
81	12.907	3672	3675	3678	rBV2	252	208	0.02%	0.003%
82	12.974	3693	3696	3699	rBV2	254	174	0.02%	0.002%
83	13.344	3807	3811	3812	rBV	380	264	0.03%	0.003%
84	13.428	3834	3837	3839	rBV	221	168	0.02%	0.002%
85	13.546	3872	3874	3878	rBV2	358	261	0.03%	0.003%
86	13.788	3946	3949	3953	rBV	428	332	0.03%	0.004%
87	14.045	4027	4029	4031	rBV	276	97	0.01%	0.001%


Sum of corrected areas: 7773527

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110720\
Data File : VV019271.D
Acq On : 05 Nov 2020 11:51
Operator : SY/MD
Sample : L4543-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

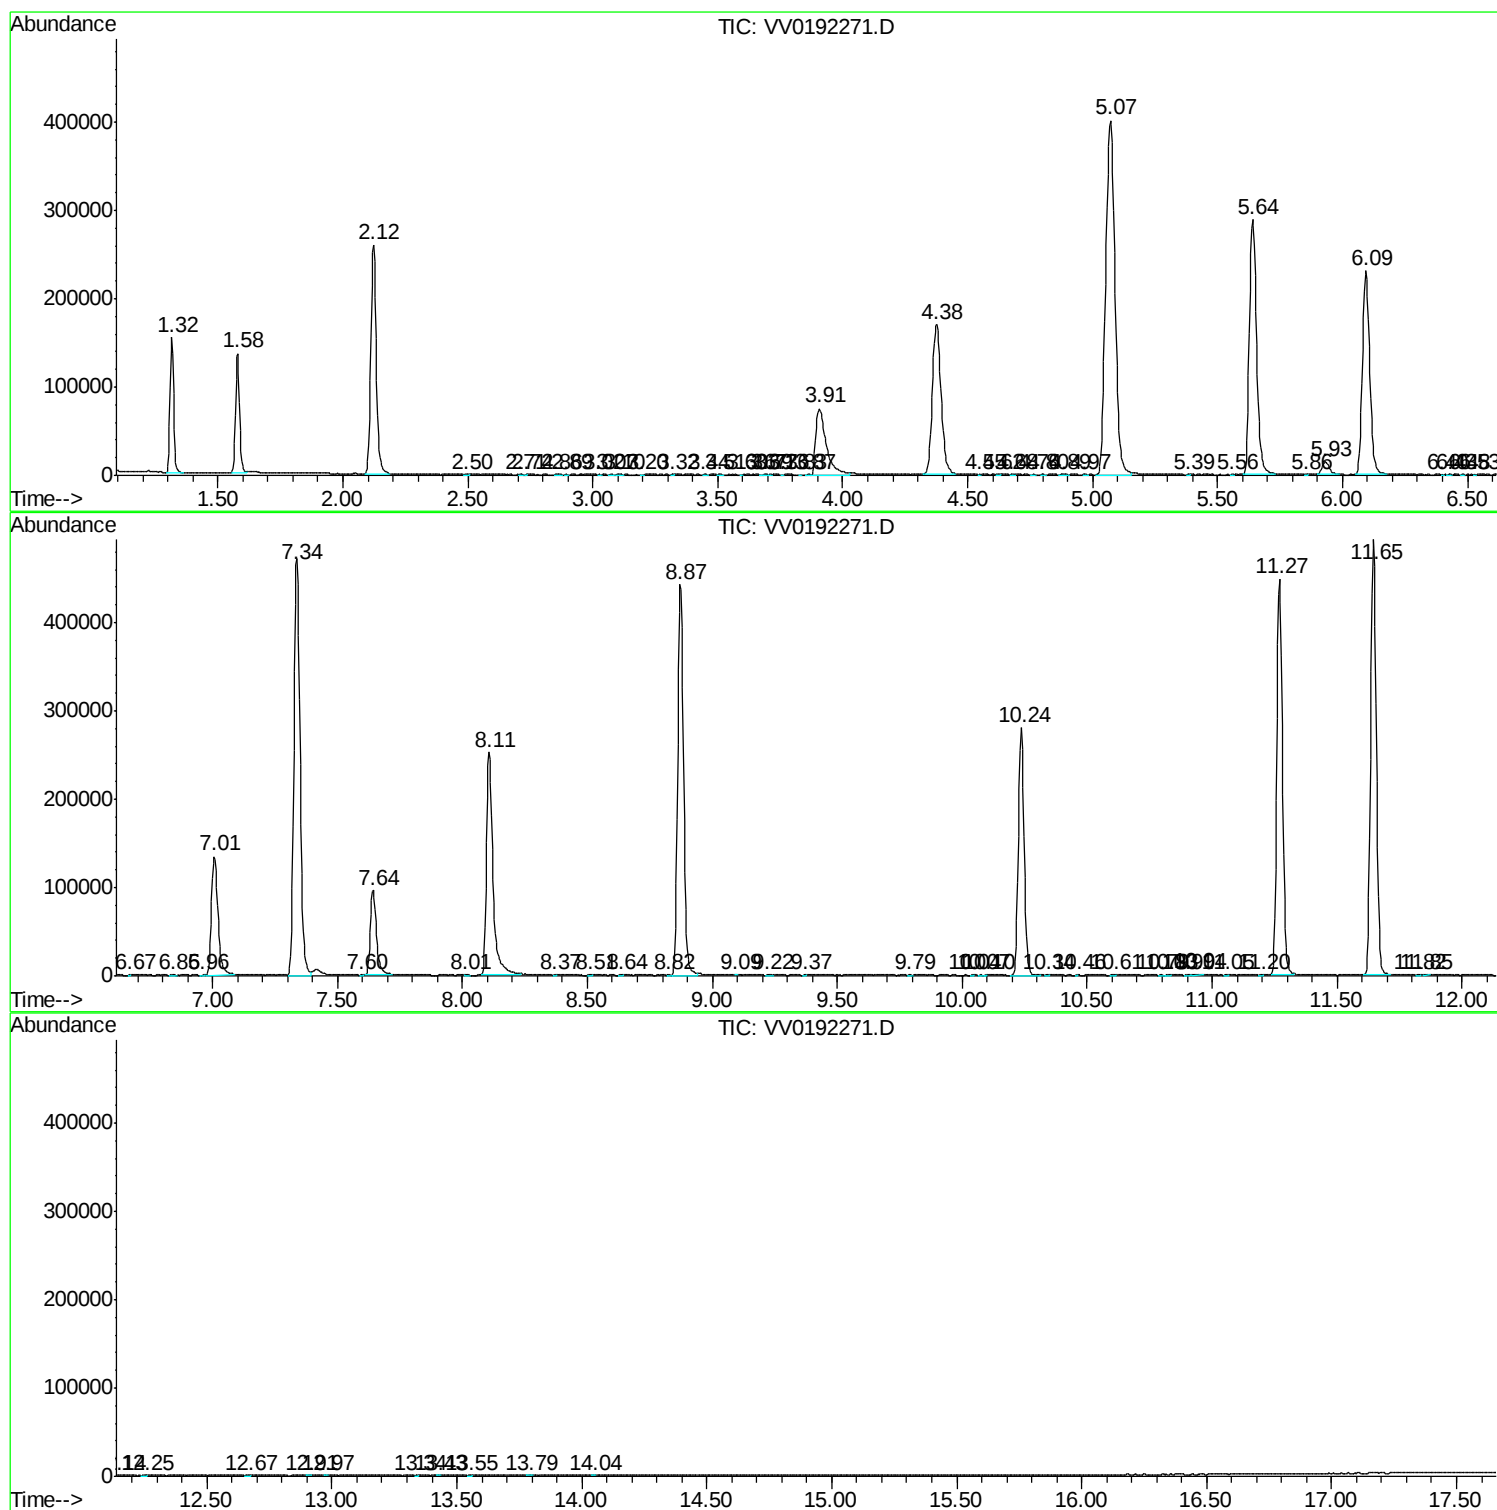

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110720\
Data File : VV019271.D
Acq On : 05 Nov 2020 11:51
Operator : SY/MD
Sample : L4543-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110720\
Data File : VV019271.D
Acq On : 05 Nov 2020 11:51
Operator : SY/MD
Sample : L4543-04
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc